

Bay Area Hydrology Model 2023

User Manual

**Prepared by
Clear Creek Solutions, Inc.
www.clearcreeksolutions.com**

**Prepared for
Alameda Countywide Clean Water Program
San Mateo Countywide Water
Pollution Prevention Program
Santa Clara Valley Urban Runoff
Pollution Prevention Program
Contra Costa Clean Water Program**

December 2023



To download the Bay Area Hydrology Model 2023
and the electronic version of this user's manual,
please go to <https://www.clearcreeksolutions.info/bahm-download-page> or
<https://ftp.clearcreeksolutions.info/ftp/public/downloads/BAHM2023/bahm2023.msi>

If you have questions about BAHM2023 or its use, please contact:
Joseph Brascher, BrascherJR@clearcreeksolutions.com

BAHM2023 TRAINING VIDEOS

Included with BAHM2023 is additional training that allows the user to learn aspects of the software quickly. These videos cover all pertinent topics of using the software and are taught by CCS hydrologists and software developers. A BAHM2023 user can access the training at this link: www.clearcreeksolutions.info/bahm-course-home

End User License Agreement

End User Software License Agreement (Agreement). By clicking on the “Accept” Button when installing the Bay Area Hydrology Model 2023 (BAHM2023) software or by using the Bay Area Hydrology Model 2023 software following installation, you, your employer, client, and associates (collectively, “End User”) are consenting to be bound by the following terms and conditions. If you or End User do not desire to be bound by the following conditions, click the “Decline” Button, and do not continue the installation process or use of the Bay Area Hydrology Model 2023 software.

The Bay Area Hydrology Model 2023 software is being provided to End User pursuant to a sublicense of a governmental licensee of Clear Creek Solutions, Inc. Pursuant to the terms and conditions of this Agreement, End User is permitted to use the Bay Area Hydrology Model 2023 software solely for purposes authorized by participating municipal, county or special district member agencies of signatory programs which are organized on a county-wide basis for implementation of stormwater discharge permits issued by the California Regional Water Quality Control Board, San Francisco Bay Region, under the National Pollutant Discharge Elimination System. The signatory programs include the Alameda Countywide Clean Water Program (ACCWP), the Santa Clara Valley Urban Runoff Pollution Prevent Program (SCVURPPP), the San Mateo Countywide Water Pollution Prevention Program (SMCWPPP), and the Contra Costa Clean Water Program (CCCWP), each of which participated in jointly funding the development of BAHM2023 and are hereinafter referred to collectively as “Participants”. The End User is not permitted to use the Bay Area Hydrology Model 2023 software for any other purpose than as described above.

End User shall not copy, distribute, alter, or modify the Bay Area Hydrology Model 2023 software.

The BAHM2023 incorporates data on soils, climate and geographical features to support its intended uses of identifying site-appropriate modeling parameters, incorporating user-defined inputs into long-term hydrologic simulation models of areas within the jurisdictions of the Participants, and assisting design of facilities for hydromodification as described in the accompanying documentation. This data may not be adequate for other purposes such as those requiring precise location, measurement or description of geographical features, or engineering analyses other than those described in the documentation.

This program and accompanying documentation are provided 'as-is' without warranty of any kind. The entire risk regarding the performance and results of this program is assumed by End User. Clear Creek Solutions Inc. and the governmental licensee or sublicensees disclaim all warranties, either expressed or implied, including but not limited to implied warranties of program and accompanying documentation. In no event shall Clear Creek Solutions Inc, EOA Inc., member agencies of ACCWP, member agencies of SMCWPPP, member agencies of SCVURPPP, members of CCCWP, or any other Participants or authorized representatives of Participants be liable for any damages whatsoever (including without limitation to damages for loss of business profits, loss of business information, business interruption, and the like) arising out of the use of, or inability to use this program even if Clear Creek Solutions Inc., EOA Inc. or any member agencies of the Participants or their authorized representatives have been advised of the possibility of such damages. Software Copyright © by Clear Creek Solutions, Inc. 2023-2024; All Rights Reserved.

FOREWORD

The Bay Area Hydrology Model 2023 (BAHM2023) is a tool for analyzing the hydromodification effects of land development projects and sizing solutions to mitigate the increased runoff from these projects. This section of the User Manual provides background information on the definition and effects of hydromodification, the regulatory history for stormwater programs in the San Francisco Bay Region, and relevant findings from technical analyses conducted in response to regulatory requirements. It also summarizes the current Hydromodification Management Standard and general design approach for hydromodification control facilities, which led to the development of the BAHM2023.¹

Effects of Hydromodification

Urbanization of a watershed modifies natural watershed and stream processes by altering the terrain, modifying the vegetation and soil characteristics, introducing pavement and buildings, installing drainage and flood control infrastructure, and altering the condition of stream channels through straightening, deepening, and armoring. These changes affect hydrologic characteristics in the watershed (rainfall interception, infiltration, runoff and stream flows), and affect the supply and transport of sediment in the stream system. The change in runoff characteristics from a watershed caused by changes in land use conditions is called *hydrograph modification*, or simply hydromodification.

As the total area of impervious surfaces increases in previously undeveloped areas, infiltration of rainfall decreases, causing more water to run off the surface as overland flow at a faster rate. Storms that previously didn't produce runoff under rural conditions can produce erosive flows. The increase in the volume of runoff and the length of time that erosive flows occur ultimately intensify sediment transport, causing changes in sediment transport characteristics and the hydraulic geometry (width, depth, slope) of channels. The larger runoff durations and volumes and the intensified erosion of streams can impair the beneficial uses of the stream channels.

Regulatory Context

The California Regional Water Quality Control Board (Water Board), San Francisco Bay Region, requires stormwater programs to address the increases in runoff rate and volume from new and redevelopment projects where those increases could cause increased erosion of receiving streams. Starting in 2002, Phase 1 municipal stormwater permits in the San Francisco Bay Area contained requirements to develop and implement hydromodification management plans (HMPs) and to implement associated management measures.

¹ Portions of this Foreword were excerpted from Bicknell, Beyerlein and Feng, "The Bay Area Hydrology Model – A Tool for Analyzing Hydromodification Effects of Development Projects and Sizing Solutions", 2006.

<https://www.semanticscholar.org/paper/The-Bay-Area-Hydrology-Model-A-Tool-for-Analyzing-Bicknell-Beyerlein/b6636d06cc31ec47fca1883b49f6b35bc90179b4>

The first Bay Area permit to include the new requirements was that of the Santa Clara Valley Urban Runoff Pollution Prevention Program (SCVURPPP). SCVURPPP conducted an assessment of hydromodification impacts on streams tributary to South San Francisco Bay and developed an HMP Report² that describes the results of the assessments and technical studies and how SCVURPPP agencies will meet the hydromodification management requirements. On July 20, 2005, the Water Board adopted key provisions of the HMP Report into SCVURPPP's permit.

Subsequently, other Bay Area countywide stormwater programs developed and began implementing HMPs in response to similar permit requirements, and those HMPs were also adopted by the Water Board.³ On October 14, 2009, the Water Board adopted a Municipal Regional Permit (MRP) that consolidated all Bay Area Phase I municipal stormwater program permit requirements into one permit. The MRP includes the current hydromodification management requirements for the individual stormwater programs⁴.

Technical Analysis of Hydromodification Controls

SCVURPPP and its consultant team completed a literature review and a number of technical analyses to address key issues for hydromodification management, such as the effectiveness of various flow control techniques, the range of storm events to be considered for design criteria, and examples of flow duration basin sizing for local projects⁵. The key findings of these analyses, which served as the basis for developing performance criteria for hydromodification controls, are described below.

Effective Design Approaches

It has been previously demonstrated that control of peak flows alone is not adequate for erosion control. SCVURPPP's studies showed that hydromodification controls designed for discrete event volume control or design storm hydrograph matching do not provide adequate protection of receiving streams. The recommended effective method for hydromodification control is *flow duration control*. This approach involves incorporating one or more flow control structures to maintain the magnitude and duration of post-project flows at the same level as the pre-project flows (i.e., matching the long-term pattern of flow rates and the proportion of time during which they occur) for the full distribution of flows within a significant range. The flow duration approach considers the entire multi-year discharge record, as opposed to a single event. Flow controls should be

² SCVURPPP, *Hydromodification Management Plan, Final Report*, April 2005.

<https://scvurppp.org/2005/04/21/hydromodification-management-plan-2/>

³The cities of Fairfield, Suisun City, Vallejo, and the Vallejo Flood & Wastewater District, which have joined together to form the Solano Stormwater Alliance, have also developed HMPs that were adopted by the Water Board; however, they currently do not use the Bay Area Hydrology Model as the basis for compliance.

⁴ For more information on the MRP, see:

https://www.waterboards.ca.gov/sanfranciscobay/water_issues/programs/stormwater/MRP/mrp5-22/R2-2022-0018.pdf

⁵ Technical memoranda describing these analyses are available in Appendix C of the SCVURPPP HMP Report.

supplemented by site design measures that reduce the amount of post-project runoff generated at the site.

Range of Storms to Manage

An evaluation was performed of the range of flows that are the most important for stream channel erosion and hydromodification impacts in Santa Clara Valley. The evaluation was based on watershed assessments conducted for three subwatersheds in the Valley. The lower limit of the range is based on the critical flow (Q_c) in each stream reach that initiates erosion of the stream bed or bank. For all three subwatersheds, Q_c could be approximated as 10% of the 2-year pre-development peak flow. To partition this allowable flow among contributing land areas, an on-site project design criteria of 10% of the pre-project 2-year peak flow was proposed, and later adopted, as the allowable low flow from a flow control facility.

The upper limit on the range of storms was determined by evaluating the contribution of different flow magnitudes to the total amount of erosive “work”⁶ done on the stream bed and banks over a period of time. The low flows contribute the most work overtime, whereas high flows contribute less work because they occur less frequently.

Approximately 90-95% of the total work on the channel boundary is done by flows between Q_c and the pre-development 10-year peak flow magnitude. Flows greater than the 10-year peak flow contribute less than 10% of the total work. Thus, the 10-year pre-project peak flow was selected as the practical upper limit for controlling erosive flows.

Hydromodification Management Standard and Design Approach

As described in current permits, the Hydromodification Management (HM) standard states that “stormwater discharges from applicable new development and redevelopment projects shall not cause an increase in the erosion potential of the receiving stream over the pre-project (existing) condition⁷. Increase in runoff flow and volume shall be managed so that post-project runoff shall not exceed estimated pre-project rates and durations, where such increased flow and/or volume is likely to cause increased potential for erosion of creek beds and banks, silt pollutant generation, or other adverse impacts to beneficial uses due to increased erosive force.” Most of the Bay Area stormwater program permits include performance and applicability criteria to meet this requirement.

Projects can meet the HM standard by use of on-site control measures, regional control measures, in-stream measures, or a combination thereof. Applicable projects with on-site flow control facilities that are designed to provide flow duration control to the pre-project condition are considered to comply with the HM standard. Flow duration controls must be designed such that post-project stormwater discharge rates and durations match pre-project discharge rates and durations from 10% of the pre-project 2-year peak flow up to the pre-project 10-year peak flow.⁸

⁶ “Work” is a measure of the erosive hydraulic forces on the stream segment in excess of what the stream bed and bank materials can withstand (critical shear stress) before sediment movement occurs.

⁷ The requirements apply to development or redevelopment projects that create and/or replace 1 acre or more of impervious surface area. Consult local stormwater programs for guidance on definition of applicable projects.

⁸ The matching criterion is as follows: the post-project flow duration curve may not deviate above the pre-project flow duration curve by more than 10% over more than 10% of the length of the curve.

On-site flow controls include site design techniques, treatment controls that have the added effect of reducing flow (normally via infiltration), and flow control structures. Examples of site design features and flow reducing treatment controls (also known as low impact development (LID) techniques) include minimizing impervious surface areas, preserving natural areas, limiting development especially where native soils have good infiltration characteristics, directing roof runoff to landscaped areas, and installing bioretention areas (landscaped treatment systems with a specified soil mix to remove pollutants). Flow control structures are generally detention/retention basins or underground vaults or tanks fitted with outlet structures such as weirs and/or orifices to control outflow rate and duration. Flow control structures can be combined with LID treatment facilities or with flood control facilities.

The basic approach for design of flow control structures to meet hydromodification requirements involves: 1) simulating the runoff from the project site under pre- and post-project conditions using a continuous simulation hydrologic model with a long-term rainfall record⁹; 2) generating flow-duration curves from the results; and 3) designing a flow control facility such that when the post-project time series of runoff is routed through the facility, the discharge pattern matches the pre-project flow-duration curve. The flow control structure is typically a type of detention facility that diverts and retains a certain portion of the runoff which is essentially the increase in surface runoff volume created between the pre-project and post-project condition. This captured increase in volume must be discharged in one of several ways: 1) to the ground via infiltration (and/or evapotranspiration if vegetation is present) in the basin; 2) released at a very low rate to the receiving stream (at the project critical flow for basin design called Q_{cp} , defined as 10% of the pre-project 2-year runoff event); and/or 3) diverted to a safe discharge location or other infiltration site, if feasible.

Development of the Bay Area Hydrology Model

The concept of designing a flow duration control facility is relatively new and, as described above, requires the use of a continuous simulation hydrologic model. To facilitate this design approach, SCVURPPP, ACCWP and SMCWPPP decided to jointly fund development of a user-friendly, automated modeling and flow duration control facility sizing software tool adapted from the Western Washington Hydrology Model (WWHM). The WWHM was developed in 2001 for the Washington State Department of Ecology to support Ecology's *Stormwater Management Manual for Western Washington*¹⁰ and assist project proponents in complying with the Western Washington hydromodification control requirements. The original Bay Area Hydrology Model (BAHM), developed in 2007, was adapted from WWHM Version 3, but has been

⁹ There are several public domain hydrologic models that can be used for simulating runoff for a continuous rainfall record and sizing flow control facilities. Examples are: 1) the Army Corps of Engineers' Hydrologic Engineering Center Hydrologic Modeling System (HEC-HMS); 2) the Environmental Protection Agency's (EPA's) Hydrologic Simulation Program Fortran (HSPF); and 3) the EPA's Stormwater Management Model (SWMM).

¹⁰ Washington State Department of Ecology. 2001. *Stormwater Management Manual for Western Washington*. Volume III: Hydrologic Analysis and Flow Control Design/BMPs. Publication No. 99-13. Olympia, WA.

calibrated to southern San Francisco Bay Area watersheds.¹¹ BAHM2013 was enhanced to be able to size other types of control measures and low impact development (LID) techniques for flow reduction as well. The latest version of the Bay Area Hydrology Model (BAHM2023) includes new tools, procedures, and methodologies incorporated in WWHM2012 and BAHM2013, as well as the inclusion of Contra Costa County data, extended precipitation and evaporation data series, and enhancements to reporting features.

BAHM2023 is a useful tool in the design process but must be used in conjunction with local design guidance to ensure compliance for specific projects. The reader should refer to Appendix D and local stormwater program guidance for additional information and suggestions for using the BAHM.

Acknowledgements

The following individuals and agencies are acknowledged for their contributions to the development of the BAHM and User Manual:

- Doug Beyerlein, Joe Brascher, Joseph Brascher Jr., and Gary Maxfield of Clear Creek Solutions, Inc., for development of WWHM and BAHM and preparation of the BAHM User Manual;
- Jill Bicknell (EOA/SCVURPPP), Arleen Feng and Jim Scanlin (ACCWP), Matt Fabry (SMCWPPP), and Fred Jarvis (EOA, Inc.) for their participation in the BAHM Oversight Committee and review of the original BAHM (2007) and User Manual;
- The following participants in the Bay Area Municipal Stormwater Collaborative's Regional BAHM Update Work Group (2022-2023):
 - SCVURPPP: Jill Bicknell (EOA), Joseph Dyke (San Jose), Rajeev Hada (Palo Alto);
 - ACCWP: Daniel Matlock and Ken Nagar (Fremont), Erwin Ching (San Leandro), Vibha Deshmukh (Pleasanton), Kan Xu (Dublin);
 - SMCWPPP: Reid Bogert (C/CAG), Krista McDonald (San Mateo County), Maziar Bozorginia (Half Moon Bay);
 - CCCWP: Erin Lennon (Contra Costa County), Yvana Hrovat (Haley & Aldrich), Tony Dubin (Dubin Environmental), Rob Dusenbury (Lotus Water)
- Anthony Donigian, AQUA TERRA Consultants, for calibration of the Alameda County watersheds and consultation on regional BAHM parameters;
- Washington State Department of Ecology for its leadership in creating the WWHM; and
- The countless municipal staff and consultants who tested BAHM, BAHM2013, and BAHM2023 and provided comments on the software.

¹¹ AQUA TERRA Consultants. 2005. Hydrologic Modeling of the Castro Valley Creek and Alameda Creek Watersheds with the U.S. EPA Hydrologic Simulation Program – FORTRAN (HSPF). Mountain View, CA.

This page has been intentionally left blank.

TABLE OF CONTENTS

End User License Agreement	iii
FOREWORD	iv
Effects of Hydromodification	iv
Regulatory Context	iv
Technical Analysis of Hydromodification Controls	v
Hydromodification Management Standard and Design Approach	vi
Development of the Bay Area Hydrology Model	vii
Acknowledgements	viii
INTRODUCTION TO BAHM2023	1
BAHM2023 OVERVIEW	3
QUICK START	5
MAIN SCREENS	35
MAP INFORMATION SCREEN.....	36
GENERAL PROJECT INFORMATION SCREEN.....	38
SCHEMATIC EDITOR.....	39
STANDARD ELEMENTS.....	41
BASIN ELEMENT	42
TRAPEZOIDAL POND ELEMENT	46
VAULT ELEMENT	51
TANK ELEMENT	53
IRREGULAR POND ELEMENT	56
GRAVEL TRENCH BED ELEMENT.....	59
SAND FILTER ELEMENT	61
CHANNEL ELEMENT.....	63
FLOW SPLITTER ELEMENT	65
TIME SERIES ELEMENT	67
SSD TABLE ELEMENT.....	68
HIGH GROUNDWATER/WETLAND ELEMENT.....	73
LID ELEMENTS	75
SELF-RETAINING AREA	76
BIORETENTION ELEMENT.....	80
IN-GROUND (INFILTRATION) PLANTER ELEMENT.....	91
FLOW-THROUGH PLANTER ELEMENT.....	94
PERMEABLE PAVEMENT ELEMENT	96
DISPERSION	99
LATERAL SOIL BASIN ELEMENT (Pervious)	102
LATERAL IMPERVIOUS AREA ELEMENT (Impervious)	104
DRY WELL ELEMENT	105
INFILTRATION TRENCH ELEMENT	107

INFILTRATION BASIN ELEMENT	109
GREEN ROOF ELEMENT	111
RAINWATER HARVESTING	113
ADDITIONAL INFORMATION.....	114
OUTLET STRUCTURE CONFIGURATIONS.....	115
INFILTRATION.....	123
AUTO POND, AUTO VAULT, AUTO TANK.....	124
STAGE-STORAGE-DISCHARGE TABLE.....	127
POINT OF COMPLIANCE.....	128
CONNECTING ELEMENTS.....	130
ANALYSIS SCREEN	134
FLOW DURATION	136
FLOW FREQUENCY	137
DRAWDOWN.....	139
HYDROGRAPHS.....	140
REPORTS SCREEN.....	142
LID ANALYSIS SCREEN.....	149
OPTIONS.....	154
DURATION CRITERIA	155
SCALING FACTORS	156
TIMESTEP	157
<i>REPORT</i>	158
<i>REVIEWER CHECKLIST</i>	165
APPENDIX A: DEFAULT BAHM2023 HSPF PERVIOUS PARAMETER VALUES FOR ALAMEDA, SAN MATEO AND CONTRA COSTA COUNTIES	172
APPENDIX B: DEFAULT BAHM2023 HSPF PERVIOUS PARAMETER VALUES FOR SANTA CLARA COUNTY	192
APPENDIX C: DEFAULT BAHM2023 HSPF IMPERVIOUS PARAMETER VALUES FOR ALAMEDA, SANTA CLARA, SAN MATEO, AND CONTRA COSTA COUNTIES	212
APPENDIX D: ADDITIONAL GUIDANCE FOR USING BAHM2023	216
Terminology and Countywide Specific Guidance.....	216
Infiltration Reduction Factor.....	219
Flow Duration Outlet Structures – Practical Design Considerations.....	219
Drawdown Time and Considerations.....	221
Additional Resources	222
APPENDIX E: BIORETENTION MODELING METHODOLOGY	224
APPENDIX F: PRECIPITATION DATA.....	230

INTRODUCTION TO BAHM2023

BAHM2023 is the Bay Area Hydrology Model Version 2023. BAHM2023 is based on the WWHM (Western Washington Hydrology Model) stormwater modeling platform. WWHM was originally developed for the Washington State Department of Ecology. More information about WWHM can be found at www.clearcreeksolutions.com. More information can be found about the Washington State Department of Ecology's stormwater management program and manual at www.ecy.wa.gov/programs/wq/stormwater/manual.html.

This user manual and development of the original BAHM, BAHM2013, and BAHM2023 were funded by the Alameda Countywide Clean Water Program (ACCWP), the Santa Clara Valley Urban Runoff Pollution Prevention Program (SCVURPPP), the San Mateo Countywide Water Pollution Prevention Program (SMCWPPP), and the Contra Costa Clean Water Program (CCCWP (BAHM2023 only)). Original HSPF calibration of Alameda watersheds were conducted by AQUA TERRA Consultants of Mountain View, CA; HSPF calibration of Santa Clara watersheds was conducted by Clear Creek Solutions. Clear Creek Solutions (the successor of the AQUA TERRA Washington state offices) is responsible for BAHM2023 and the BAHM2023 User Manual.

This user manual is organized to provide the user an example of a standard application using BAHM2023 (described in *Quick Start*) followed by descriptions of the different components and options available in BAHM2023. Appendices A through C provide a full list of the HSPF parameter values used in BAHM2023. Appendix D contains additional guidance and recommendations by the stormwater programs that have sponsored the BAHM2023 development. Appendix E contains additional guidance regarding bioretention facilities.

Throughout the user manual notes using this font (sans-serif italic) alert the user to actions or design decisions for which guidance must be consulted that is external to the BAHM2023 software, either provided in Appendix D of this user manual, at the BAHM website, or by the local municipal permitting agency.

Purpose

The purpose of BAHM2023 is to size hydromodification management or flow control facilities to mitigate the effects of increased runoff (peak discharge, duration, and volume) from proposed land use changes that impact natural streams, wetlands, and other water courses.

BAHM2023 provides:

- A uniform methodology for four San Francisco Bay Area counties
- A more accurate methodology than single-event design storms
- An easy-to-use software package

BAHM2023 is based on:

- Continuous simulation hydrology (HSPF)
- Actual long-term recorded precipitation data
- Measured pan evaporation data
- Existing vegetation (for pre-project conditions)
- Regional HSPF parameters

NOTE: Because of changes in input format and software architecture, original (2007) BAHM project files cannot be read or used by BAHM2023. BAHM2013 project files can be read by BAHM2023, but BAHM2023 may produce different results due to its extended precipitation data records.

What's New in BAHM2023

BAHM2023 gives the user greater modeling flexibility, options, and accuracy than were available in the original BAHM (dated 2007). The original BAHM included some simplified approaches to modeling stormwater LID (low impact development) facilities. BAHM2013 and BAHM2023 include modeling elements that more accurately represent these stormwater facilities.

Specific changes and additions in BAHM2023 include:

- Ability to run on Microsoft Windows 11 operating systems or later either on a workstation (single computer) or network.
- Updated rain gage data for the included jurisdictions and counties (extended to the end of Water Year 2021).
- Updated defaults to the Bioretention element.
- Added Contra Costa County area map, and rainfall and evaporation data.
- Description of Self-Retaining Area modeling approach.
- Additional Impervious Area options.
- Description of the use of Simple Bioretention
- Additional Riser and Weir representations.

Computer Requirements

- Windows 7/8/10/11 with 200 MB uncompressed hard drive space
- Internet access (only required for downloading BAHM2023, not required for executing BAHM2023)
- Pentium 3 or faster processor (desirable)
- Color monitor (desirable)

Requirements Before Starting the Program

- Knowledge of the site location and/or street address.
- Knowledge of the actual distribution of existing site soil by category (A, B, or C/D).
- Knowledge of the planned distribution of the proposed development (buildings, streets, sidewalks, parking, lawn areas) overlying the soil categories.

BAHM2023 OVERVIEW

The BAHM2023 software architecture and methodology is the same as that developed for the WWHM and uses HSPF as its computational engine¹². Like WWHM, BAHM2023 is a tool that generates flow duration curves for the pre- and post-project condition and then sizes a flow duration control basin or vault and outlet structure to match the pre-project curve. The software package consists of a user-friendly graphical interface with screens for input of pre-project and post-project conditions; an engine that automatically loads appropriate parameters and meteorological data and runs continuous simulations of site runoff to generate flow duration curves; a module for sizing or checking the control measure to achieve the hydromodification control standard; and a reporting module.

The HSPF hydrology parameter values used in BAHM2023 are based on calibrated watersheds located in the San Francisco Bay Area: two Alameda County watersheds and two Santa Clara County watersheds. BAHM2023 uses one or more long-term local precipitation gages for each of four San Francisco Bay counties and then scales the precipitation to the user's site using mean annual precipitation maps developed by local flood control districts or published as NOAA rainfall maps.

BAHM2023 computes stormwater runoff for a site selected by the user. BAHM2023 runs HSPF in the background to generate an hourly runoff time series from the available rain gage data over a number of years. Stormwater runoff is computed for both pre-project and post-project land use conditions. Then, another part of the BAHM2023 routes the post-project stormwater runoff through a stormwater control facility of the user's choice.

BAHM2023 uses the pre-project peak flood value for each water year to compute the pre-project 2- through 50-year flood frequency values¹³. The post-project runoff 2- through 50-year flood frequency values are computed at the outlet of the proposed stormwater facility. The model routes the post-project runoff through the stormwater facility. As with the pre-project peak flow values, the maximum post-project flow value for each water year is selected by the model to compute the developed 2- through 50-year flood frequency.

The pre-project two-year peak flow is multiplied by 10% to set the lower limit of the erosive flows, in accordance with the current hydromodification management (HM) performance criteria¹⁴. The pre-project 10-year peak flow is the upper limit. A comparison of the pre-project and post-project flow duration curves is conducted for 100 flow levels between the lower limit and the upper limit. The model counts the number of hours that pre-project flows exceed each of the flow levels during the entire simulation period. The model does the same analysis for the post-project mitigated flows.

¹² BAHM2023 is based on WWHM Version 2012.

¹³ The actual flood frequency calculations are made using the Weibull ranking procedure.


¹⁴ In BAHM2023, this low flow limit is a user-defined variable, to allow flexibility pending potential changes in regulatory requirements.

Low impact development (LID) practices have been recognized as opportunities to reduce and/or eliminate stormwater runoff at the source. They include compost-amended (engineered) soils, bioretention, permeable pavement, green roofs, rain gardens, and infiltration trenches. All of these approaches reduce stormwater runoff. BAHM2023 can be used to determine the magnitude of the reduction from each of these practices and the amount of stormwater detention storage still required to meet HM requirements.

QUICK START


Quick Start very briefly describes the steps to quickly size a stormwater detention pond using BAHM2023. New users should read the descriptions of the BAHM2023 screens, elements, and analysis tools before going through the steps described below.

1. Select the county in which the project site is located.

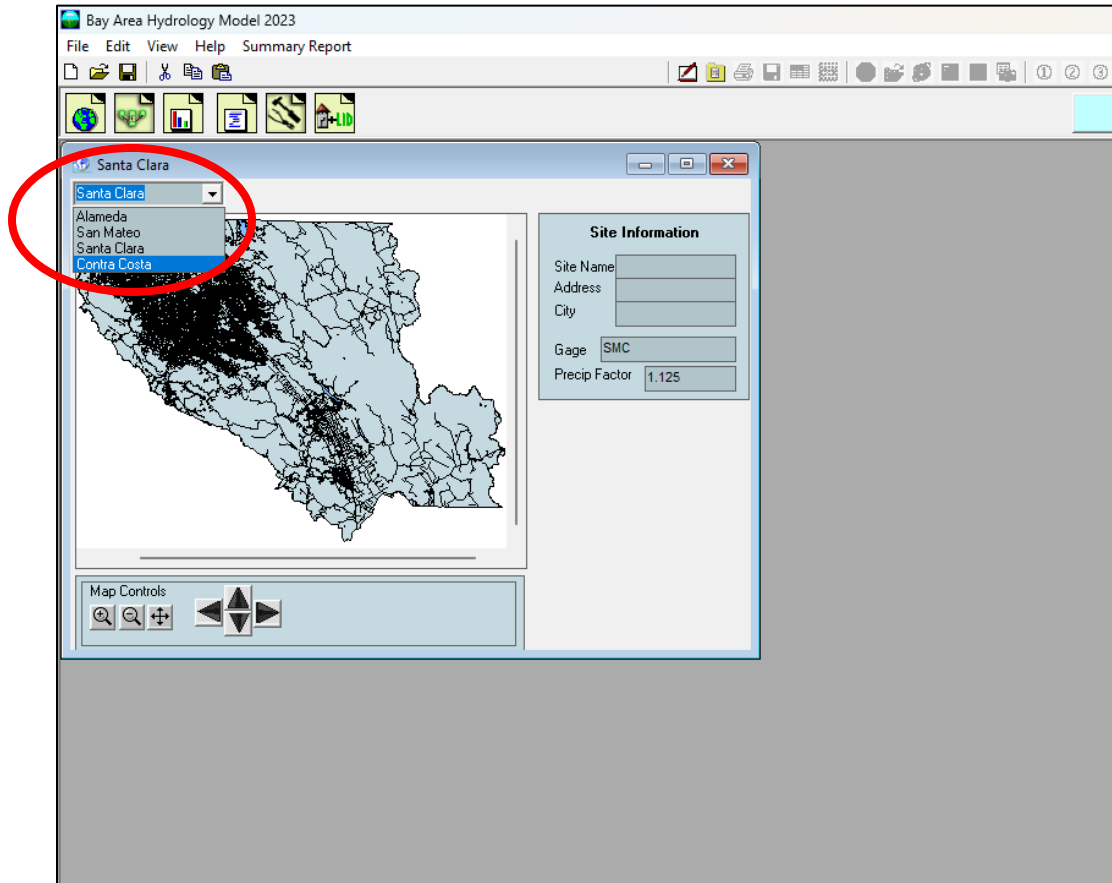

Click the down arrow in the box in the upper left corner. A list of the counties is shown. Scroll down to find the county you want. Left click on the county name. The county map will then show on the map screen.


Locate the project site on the map. Use the map controls to magnify a portion of the map, if needed. Select the project site by left clicking on the map location. A red square will be placed on the map identifying the project site.

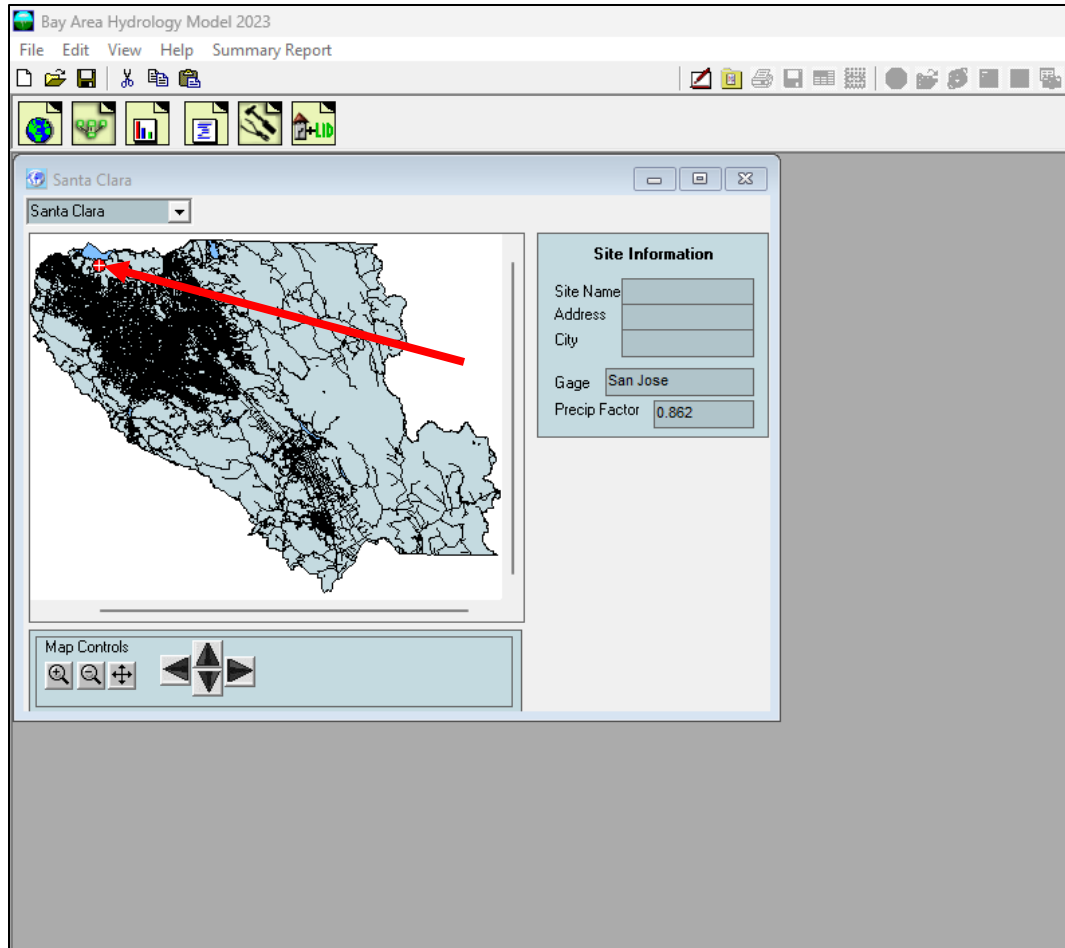

The BAHM2023 selects the appropriate rain gage record and precipitation multiplication factor. Note that for this example the rain gage is San Jose, and the precipitation multiplication factor is 0.862.

The precipitation multiplication factor is the ratio of the project site mean annual precipitation to that of the nearest precipitation station included in BAHM2023. In the above example a factor of 0.862 indicates that the mean annual precipitation of the project site is 86.2% of the mean annual precipitation of the San Jose station. BAHM2023 automatically computes the precipitation multiplication factor based on mean annual precipitation data included in its database.

2. Use the tool bar (immediately above the map) to move to the Scenario Editor. Click on the General Project Information button.



The General Project Information button will bring up the Schematic Editor.


The schematic editor screen contains two scenarios: Pre-project and Mitigated.


Set up first the Pre-project scenario and then the Mitigated scenario.

Check the Pre-project scenario box.

Left click on the Basin element under the Elements heading. The Basin element represents the project drainage area. It is the upper left element.

Select any grid cell (preferably near the top of the grid) and left click on that grid. The basin will appear in that grid cell.

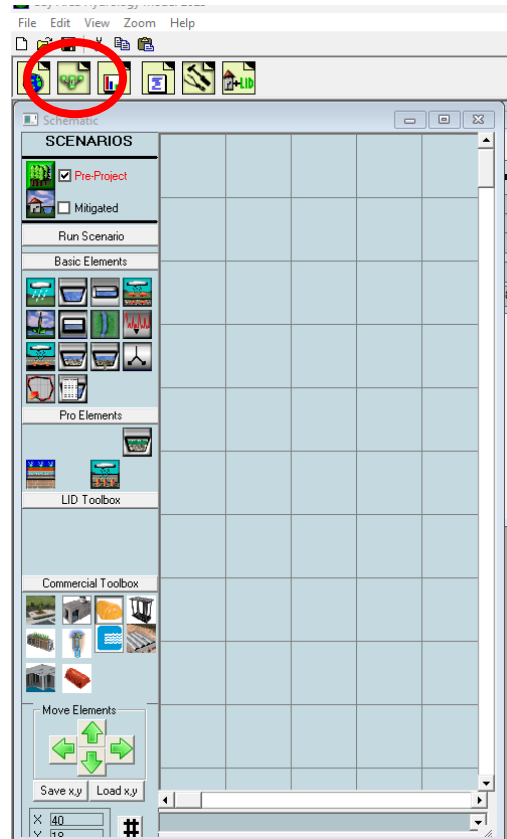

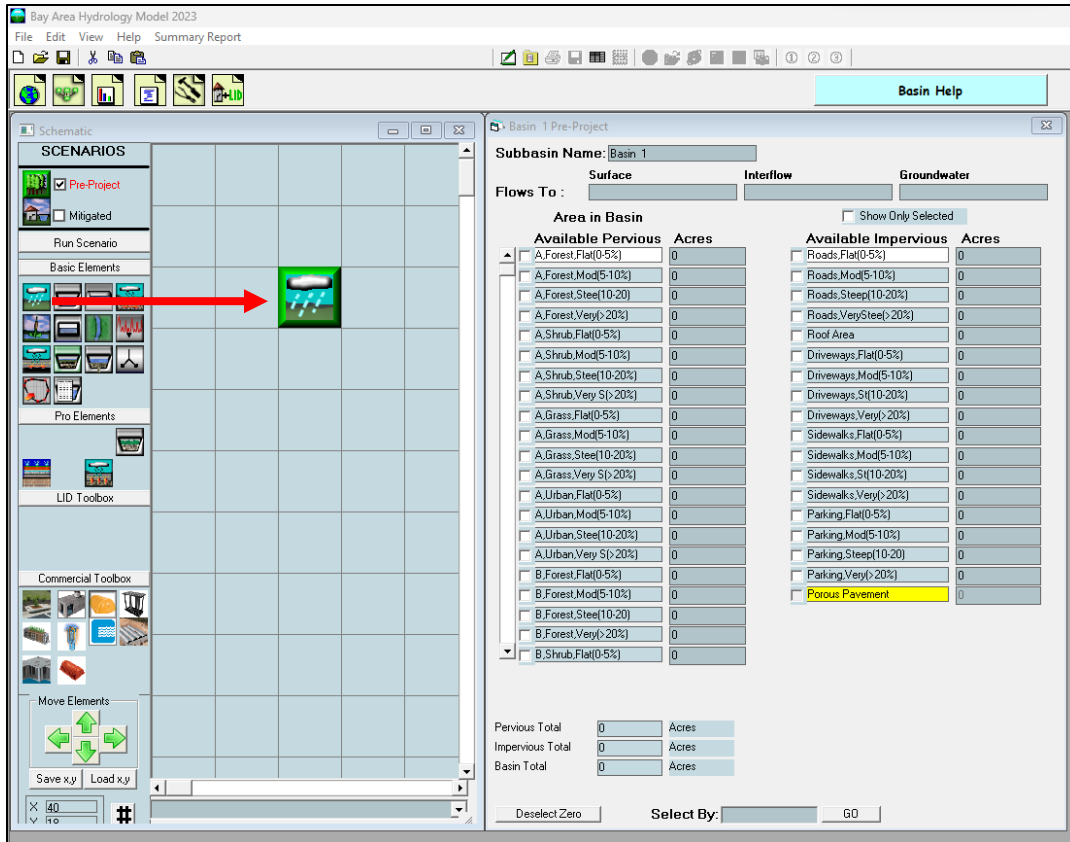


To the right of the grid is the land use information associated with the basin element. Select the appropriate soil, vegetation, and land slope for the Pre-project scenario. Soils are based on NRCS general categories A, B, C, and D (for modeling purposes BAHM2023 combines C and D into a single C/D).

Vegetation is based on the native or existing vegetation for the Pre-project area and the planned vegetation for the planned development (Mitigated scenario). Non-urban vegetation has been divided into forest, shrub, and non-turf grass and refers to the natural (non-planted) vegetation. In contrast, the developed landscape will consist of irrigated urban vegetation (lawns, flowers, planted shrubs and trees).

Land slope is divided into flat (0-5%), moderate (5-10%), steep (10-20%), and very steep (>20%) land slopes.


HSPF parameter values in BAHM2023 have been adjusted for the different soil, vegetation, and land slope categories.

For this example, we will assume that the Pre-project land use is 10 acres of D soil with non-turf grass vegetation on a steep slope (10-20%) and 1 acre of pre-project impervious area on a flat (0-5%) slope.

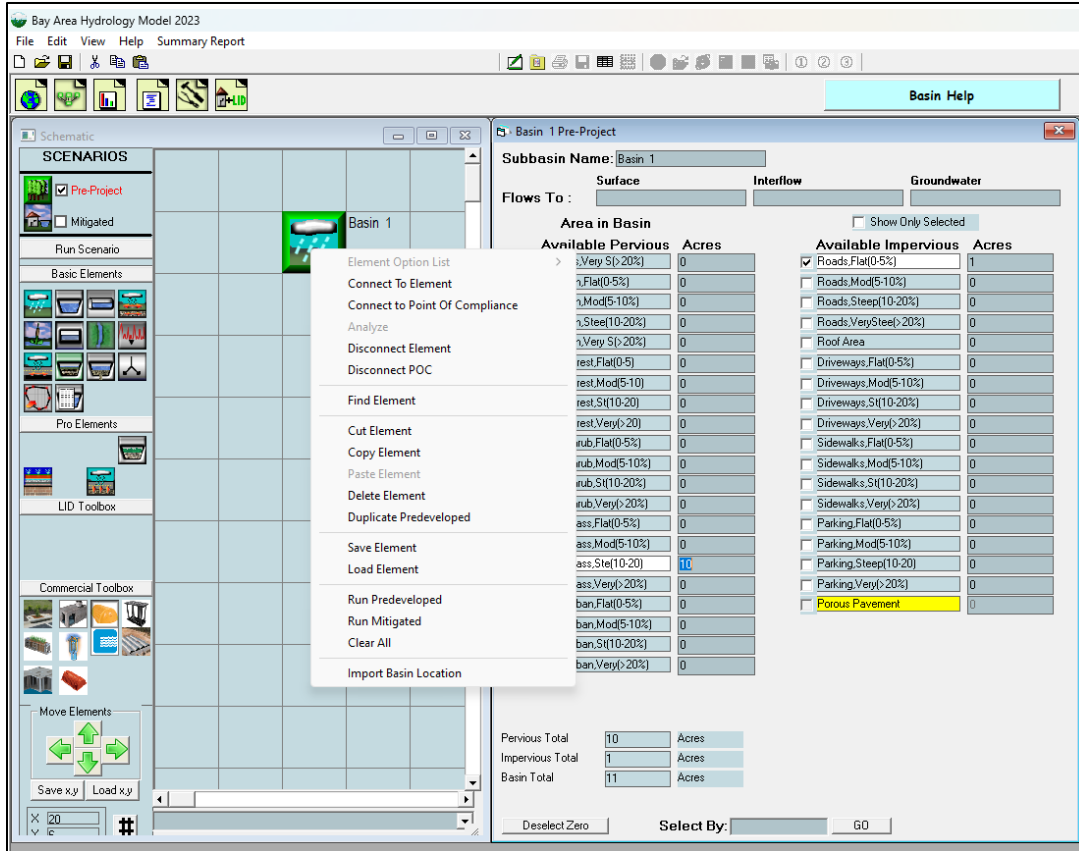


The exit from this basin will be selected as our point of compliance for the Pre-project scenario. Right click on the basin element and highlight Connect to Point of Compliance (the point of compliance is defined as the location at which the runoff from both the Pre-project scenario and the Mitigated scenario are compared).

The Point of Compliance screen will be shown for Pre-project Basin 1. The POC (Point of Compliance) outlet has been checked for both surface runoff and interflow (shallow subsurface flow). These are the two flow components of stormwater runoff. Do not check the groundwater box unless there is observed and documented base flow on the project site.

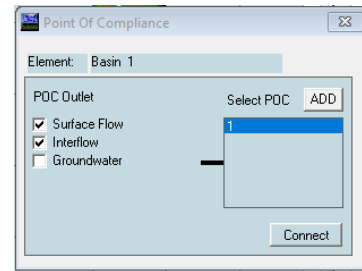


Click the Connect button in the low right corner to connect this point of compliance to the Pre-project basin.

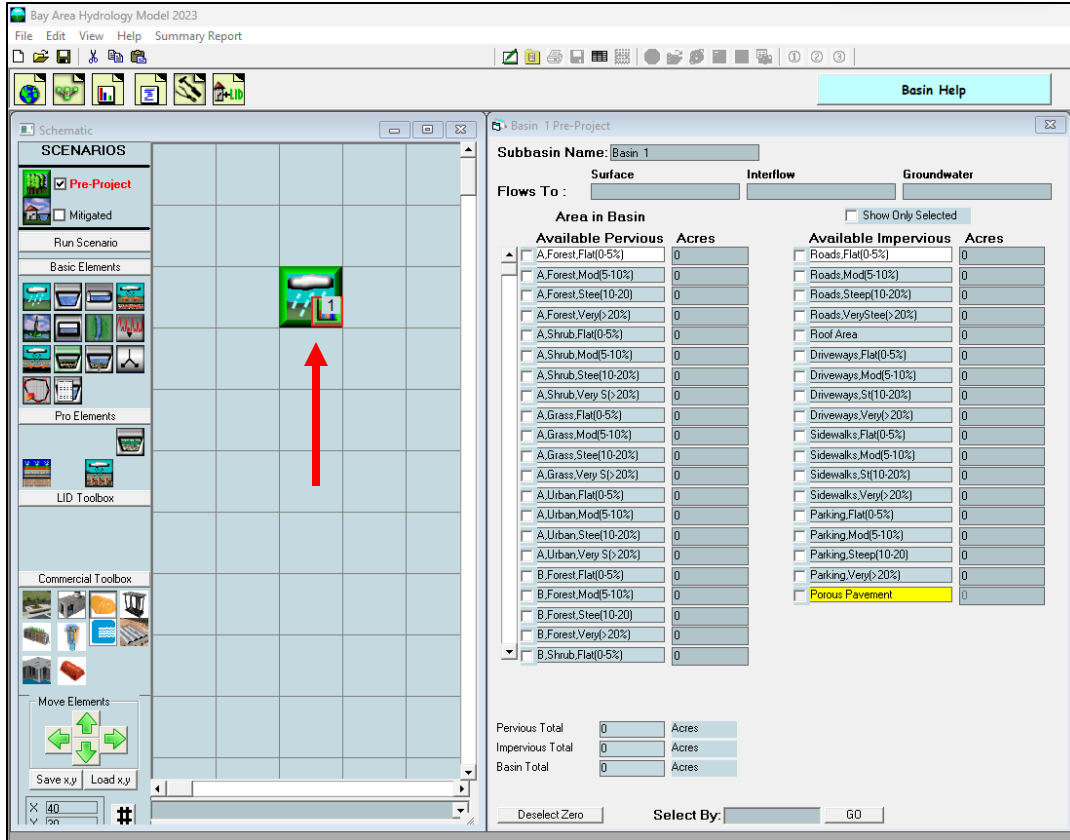


After the point of compliance has been added to the basin the basin element will change. A small box with a bar chart graphic and a number will be shown in the lower right corner of the basin element. This small POC box identifies this basin as a point of compliance. The number is the POC number (e.g., POC 1).

3. Set up the Mitigated (i.e., Post-Project) scenario.

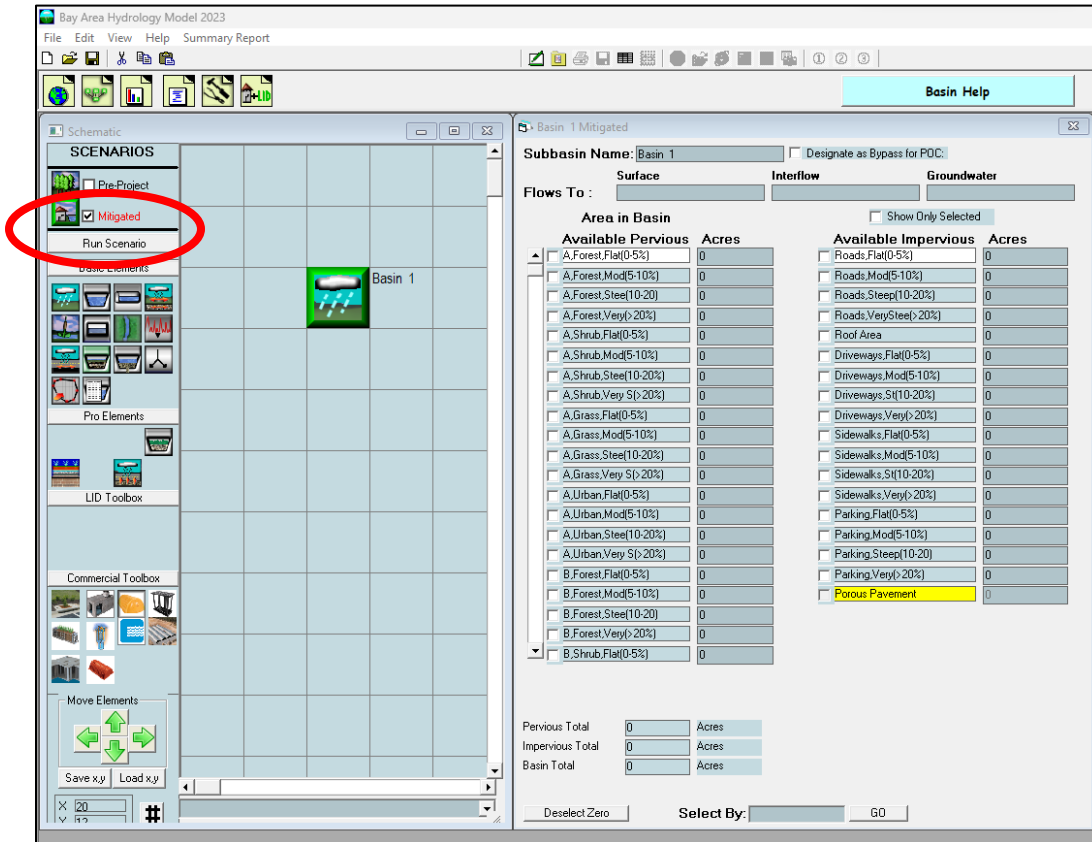

First, check the Mitigated scenario box and place a basin element on the grid.

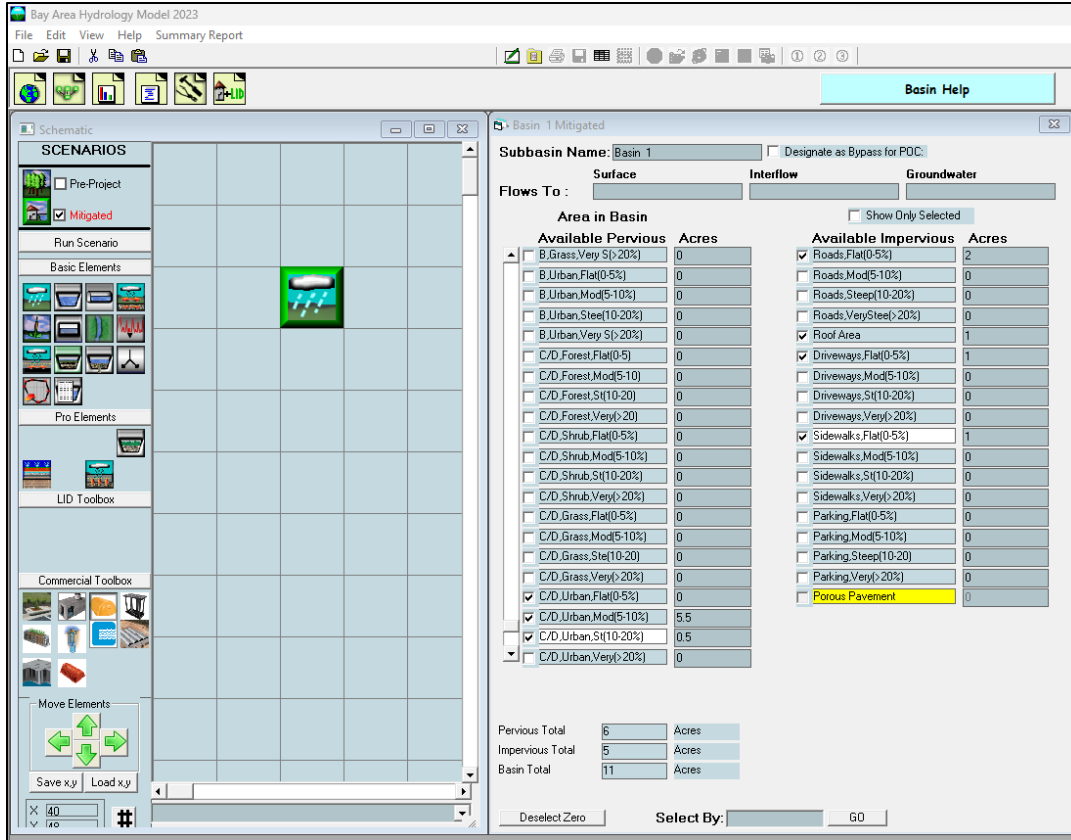


For the Mitigated land use we have:


- 5.5 acres of C/D soil, urban vegetation, moderate slope
- 0.5 acres of C/D soil, urban vegetation, steep slope
- 2 acres of roads, flat
- 1 acre of roof area
- 1 acre of driveways, flat
- 1 acre of sidewalks, flat

We will add a trapezoidal pond downstream of the basin.


The impervious land categories are roads, roofs, sidewalks, parking, and driveways. All are modeled the same, except that steeper slopes have less surface retention storage prior to the start of surface runoff.

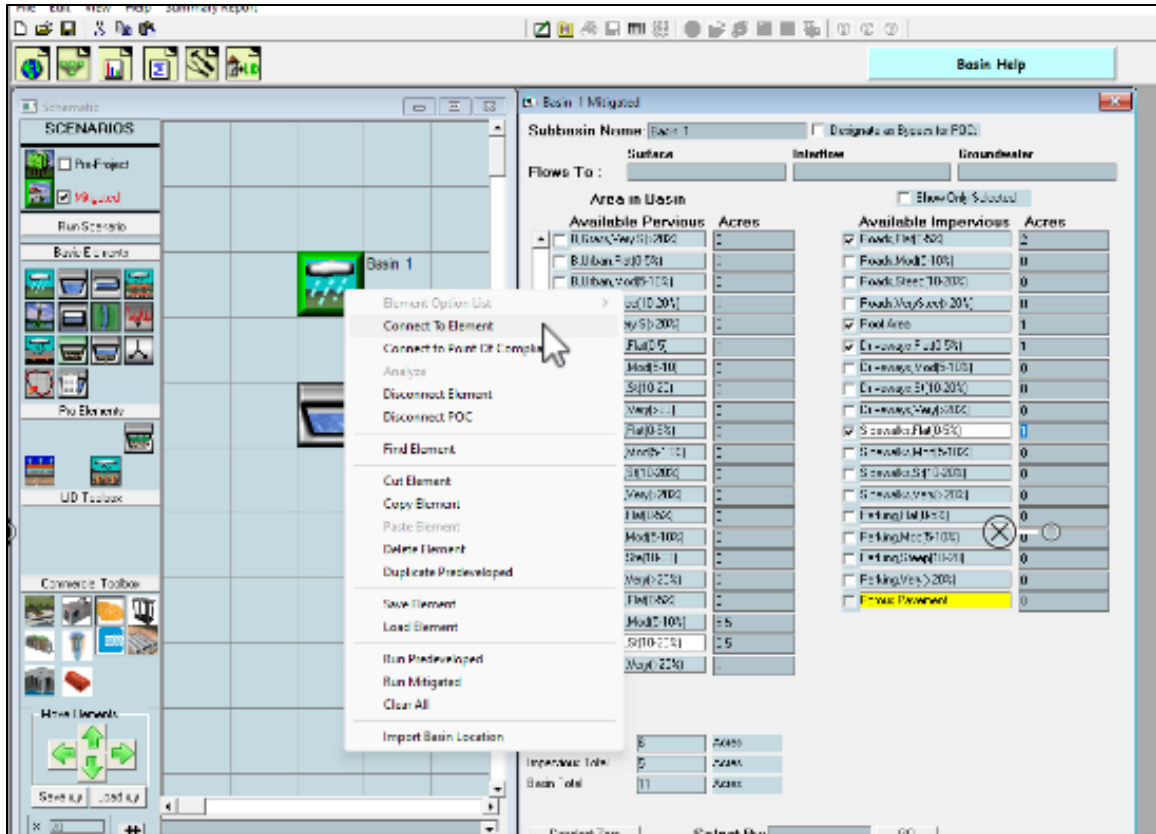


The trapezoidal pond element is placed below the basin element on the grid. Right click on the basin and select Connect To Element. A green line will appear with one end connected to the basin.

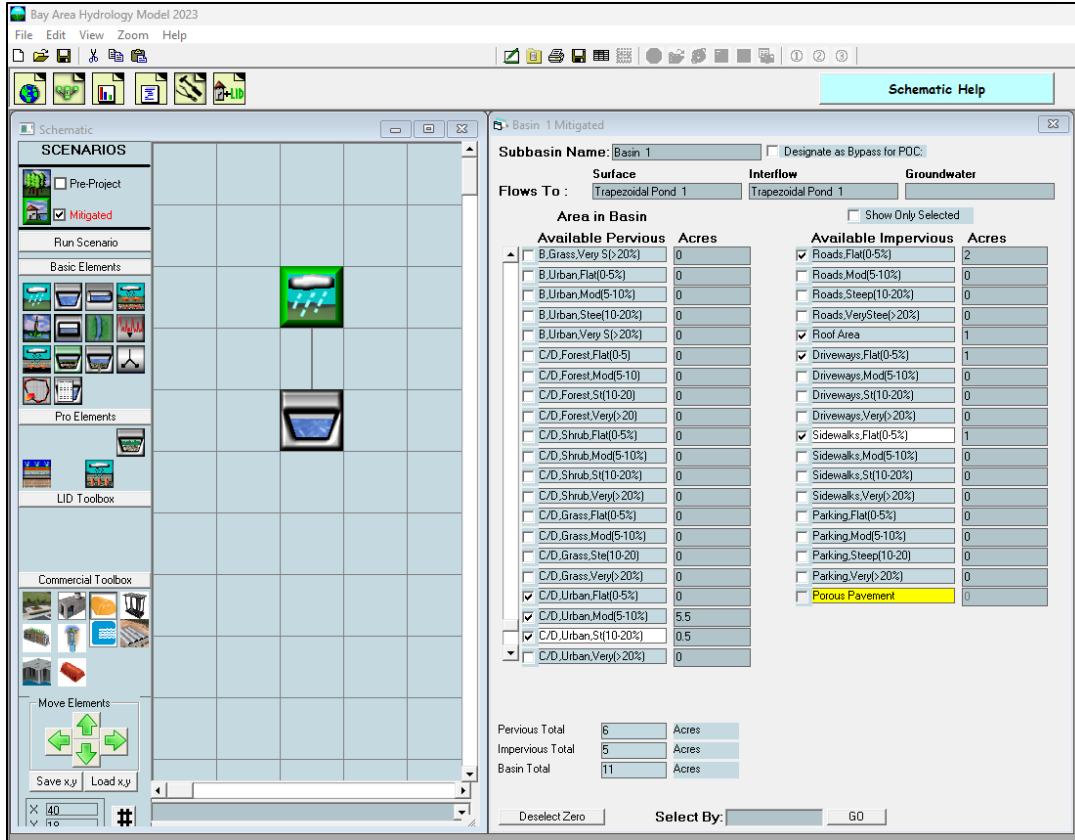


With the mouse pointer pull the other end of the line down to the trapezoidal pond and click on the pond. This will bring up the From Basin to Conveyance screen. As with the Pre-project scenario we want to only connect the surface flow and the interflow (shallow subsurface runoff) from the basin to the pond. Click OK.

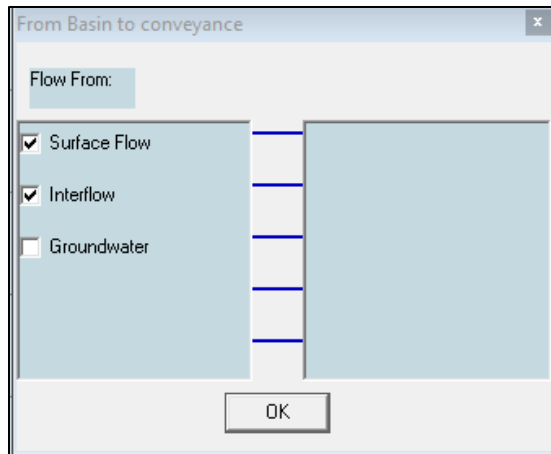


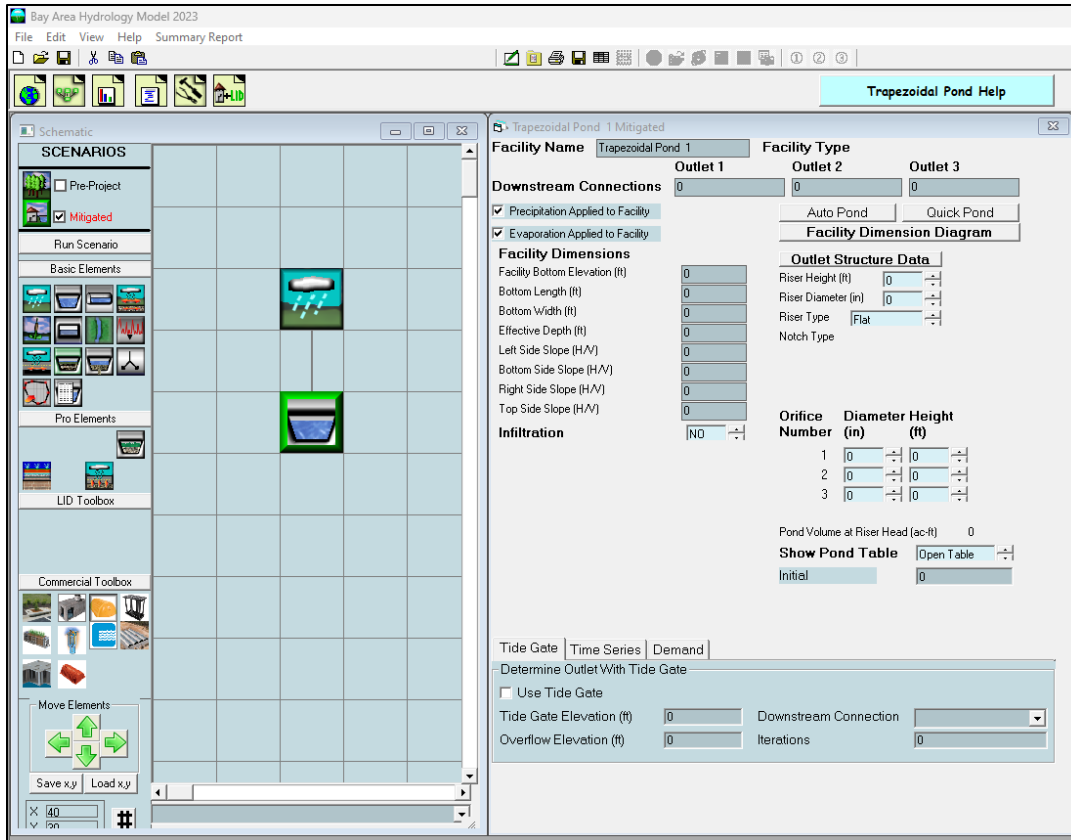


A line will connect the basin to the pond.

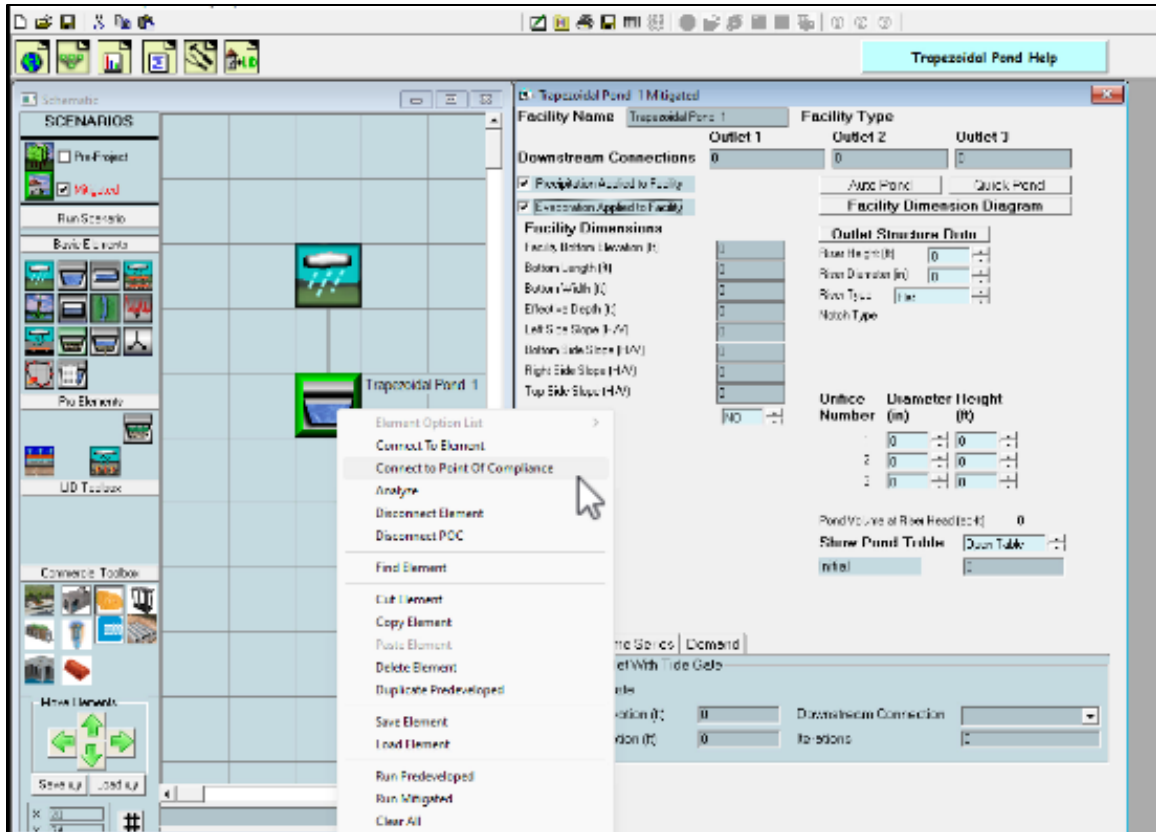

Right click on the trapezoidal pond element to connect the pond’s outlet to the point of compliance. Highlight Connect to Point Of Compliance and click.

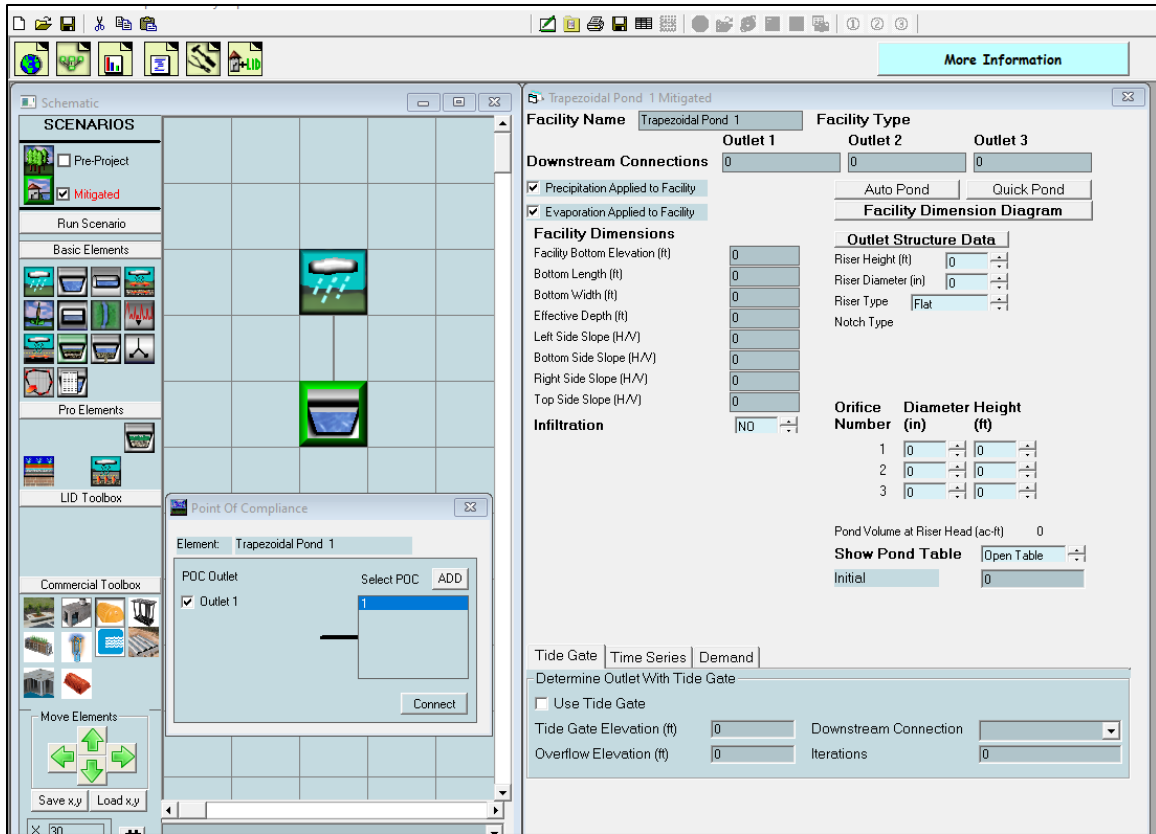


The Point of Compliance screen will be shown for the pond. The pond has one outlet (by default). The outflow from the pond will be compared with the Pre-project runoff. The point of compliance is designated as POC 1 (BAHM2023 allows for multiple points of compliance). Click on the Connect button.

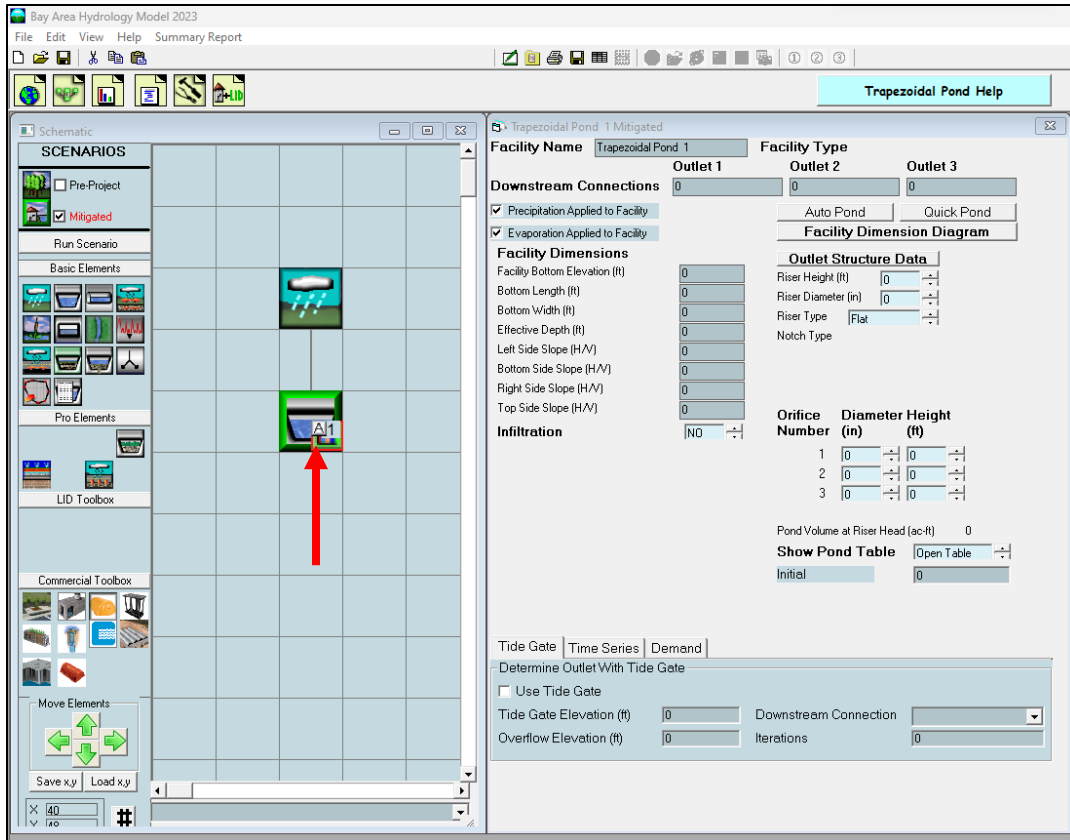

The point of compliance is shown on the pond element as a small box with the letter “A” and number 1 in the bar chart symbol in the lower right corner.

The letter “A” stands for Analysis and designates that this is an analysis location where flow and stage will be computed, and the output flow and stage time series will be made available to the user. The number 1 denotes that this is POC 1.


4. Sizing the pond.

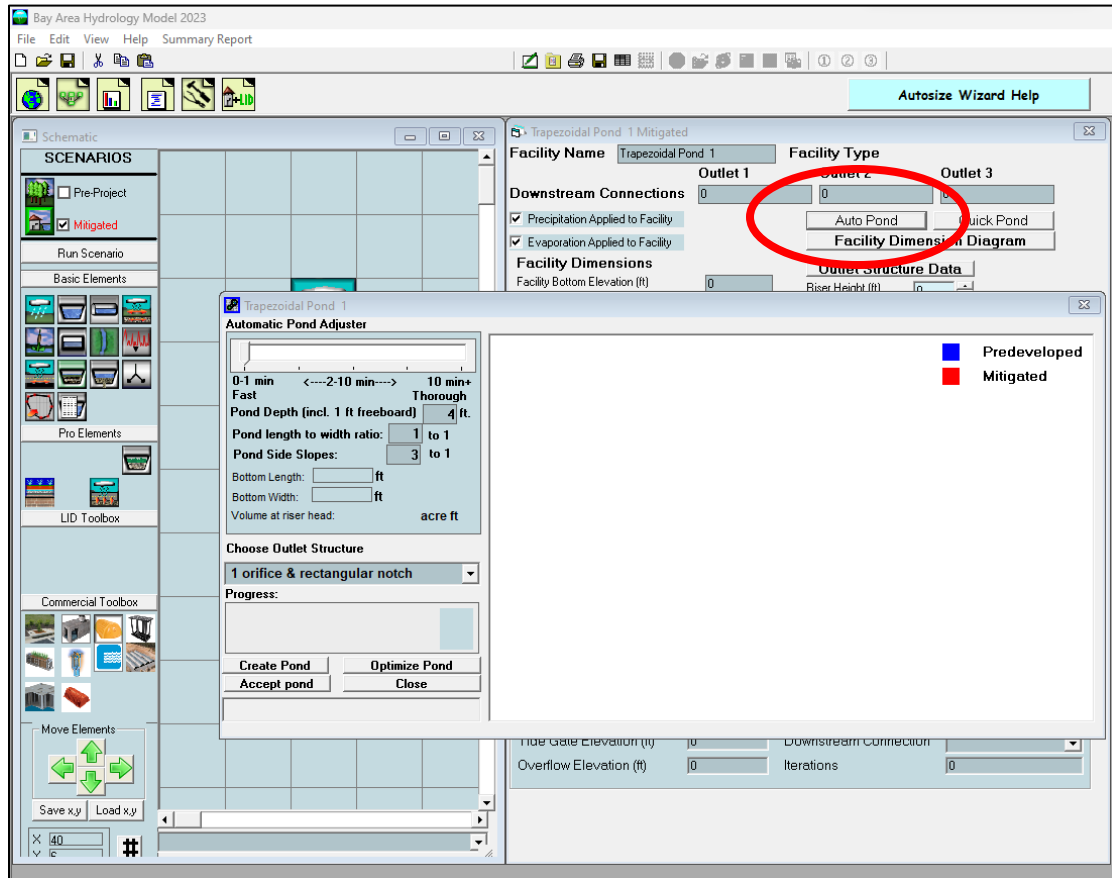

A trapezoidal stormwater pond can be sized either manually or automatically (using Auto Pond). For this example, Auto Pond will be used. (Go to page 46 to find more information about how to manually size a pond or other HM facility).

Click on the Auto Pond button and the Auto Pond screen will appear. The user can set the pond depth (default: 4 feet), pond length to width ratio (default: 1 to 1), pond side slopes (default: 3 to 1), and the outlet structure configuration (default: 1 orifice and riser with rectangular notch weir).

To optimize the pond design and create the smallest pond possible, move the Automatic Pond Adjuster pointer from the left to the right.

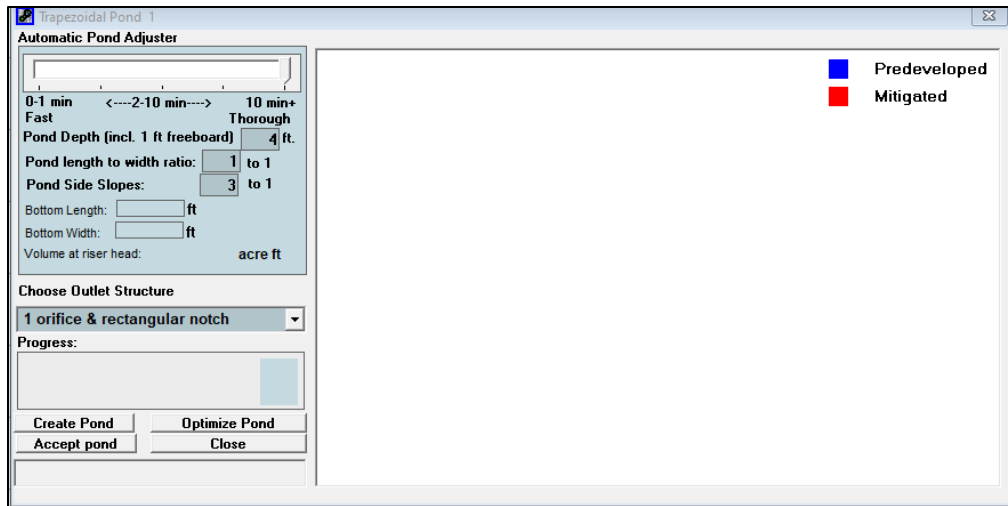

The pond does not yet have any dimensions. Auto Pond will create its own initial dimensions and then will adjust them as it goes through the automated optimization process to calculate the pond size and outlet structure dimensions.

Running Auto Pond automates the following BAHM2023 processes:

1. the hourly Pre-project runoff is computed for the 35-50 years of record (it varies depending on which rain gage is used),
2. the Pre-project runoff flood frequency is calculated based on annual peak flows,
3. the range of flows is selected for the flow duration (the default is 10% of the 2-year peak to the 10-year peak),
4. this flow range is divided into 100 increments, and
5. the number of hourly Pre-project flow values that exceed each flow increment level (Pre-project flow duration) are counted to create the flow duration curves and accompanying tabular results.


Next, BAHM2023 computes the post-project runoff (in the Mitigated scenario) and routes the runoff through the pond. But before the runoff can be routed through the pond the pond must be given dimensions and an outlet configuration. Auto Pond uses a set of rules based on the Pre-project and Mitigated scenario land uses to give the pond an initial set of dimensions and an initial outlet orifice diameter and riser (the riser is given a default rectangular notch). This information allows BAHM2023 to compute a stage-storage-discharge table for the pond.

With this initial pond stage-storage-discharge table BAHM2023:

1. routes the hourly post-project runoff through the pond for the 35-50 years of record to create to the Mitigated flow time series,
2. counts the number of hourly Mitigated flow values that exceed each flow increment level (this is the Mitigated flow duration), and

3. computes the ratio of Mitigated flow values to Pre-project flow values for each flow increment level (comparing the Pre-project and Mitigated flow duration results).

If any of the 100 individual ratio values is greater than allowed by the flow duration criteria, then the pond fails to provide an appropriate amount of mitigation and needs to be resized.

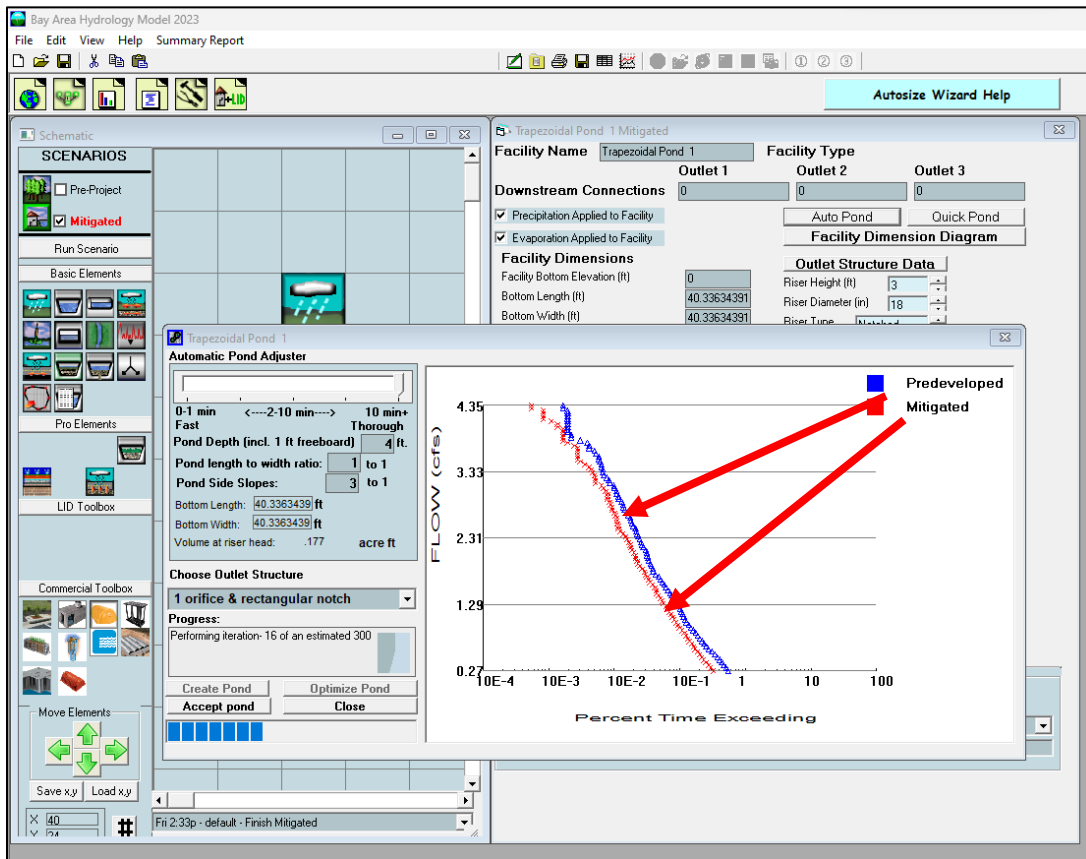


Flow duration results are shown in the plots above. The vertical axis shows the range of flows from 10% of the 2-year flow (0.27 cfs) to the 10-year flow (4.35 cfs). The horizontal axis is the percent of time that flows exceed a flow value. Plotting positions on the horizontal axis typical range from 0.001% to 1%, as explained below.

For the entire 35- to 50-year simulation period (depending on the period of record of the precipitation station used) all of the hourly time steps are checked to see if the flow for that time step is greater than the minimum flow duration criteria value (0.27 cfs, in this example). For a 50-year simulation period there are approximately 400,000 hourly values to check. Many of them are zero flows. The 10% of the Pre-project 2-year flow value is exceeded less than 1% of the total simulation period.

This check is done for both the Pre-project flows (shown in blue on the screen) and the Mitigated flows (shown in red).


If all of the Mitigated flow duration values (in red) are to the left of the Pre-project flow duration values (in blue) then the pond mitigates the additional erosive flows produced by the development.

If the Mitigated flow duration values (in red) are far to the left of the Pre-project flow duration values (in blue) then the pond can be made smaller and still meet the flow duration criteria.

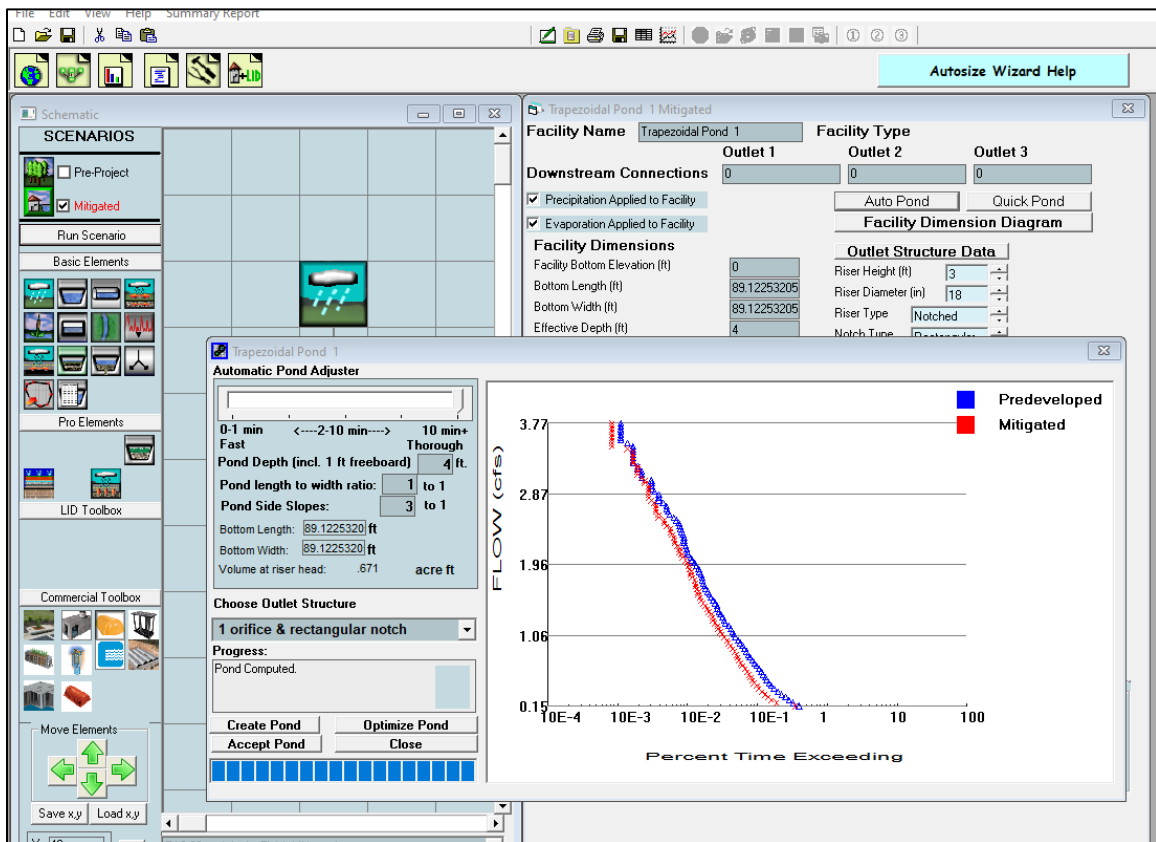

Auto Pond goes through an iteration process by which it changes the pond dimensions and outlet configuration, then instructs BAHM2023 to again compute the resulting Mitigated runoff, compare flow durations, and decide if it has made the results better or worse. This iteration process continues until Auto Pond finally concludes that an optimum solution has been found and the Mitigated flow duration values (in red) are as close as possible to the Pre-project flow duration values (in blue).


The user may continue to manually optimize the pond by manually changing pond dimensions and/or the outlet structure configuration. (Manual optimization is explained in more detail on page 46). After making these changes the user can click on the Optimize Pond button to check the results and see if Auto Pond can make further improvements.

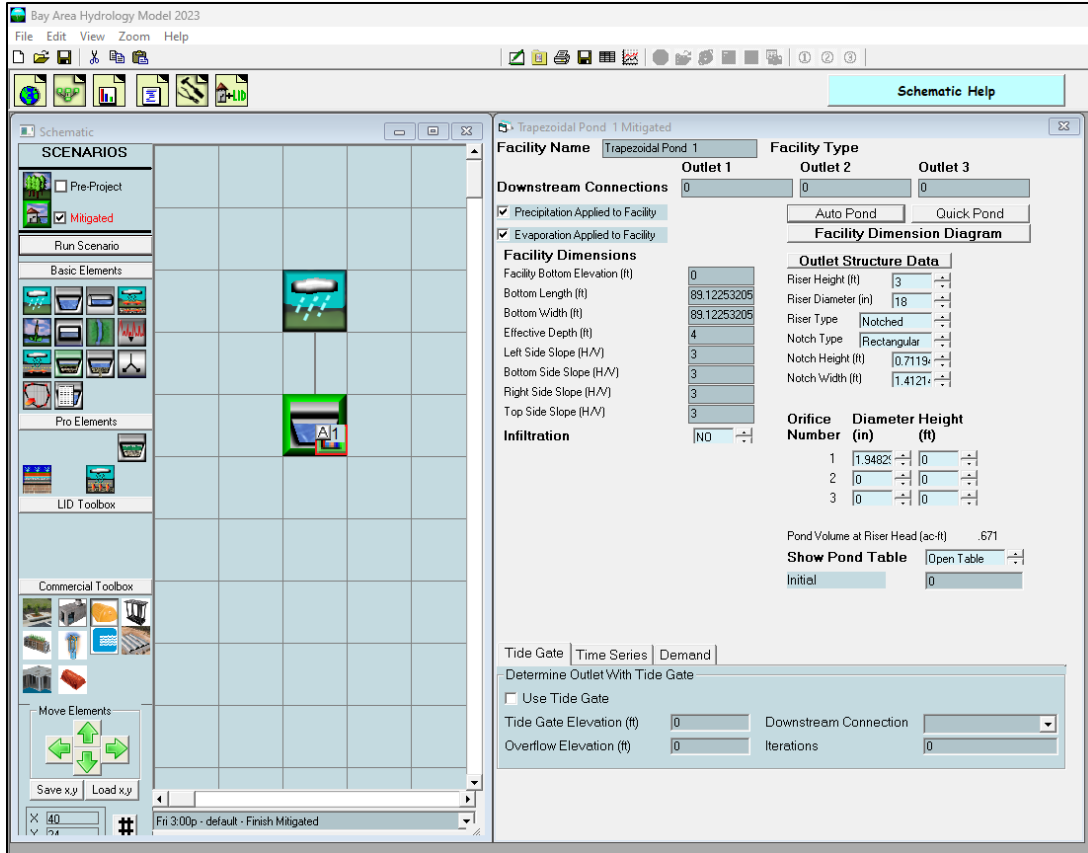


The final pond dimensions (bottom length, bottom width, effective pond depth, and side slopes) and outlet structure information (riser height, riser diameter, riser weir type, weir notch height and width, and orifice diameter and height) are shown on the trapezoidal pond screen to the right of the Schematic grid.

NOTE: If Auto Pond selects a bottom orifice diameter smaller than the smallest diameter allowed by the local municipal permitting agency then the user has the option of specifying a minimum allowable bottom orifice diameter even if this size diameter is too large to meet flow duration criteria for this element. Additional mitigating BMPs may be required to meet local hydromodification control requirements. Please see Appendix D or consult with local municipal permitting agency for more details. For manual sizing information see page 46.


5. Review analysis.

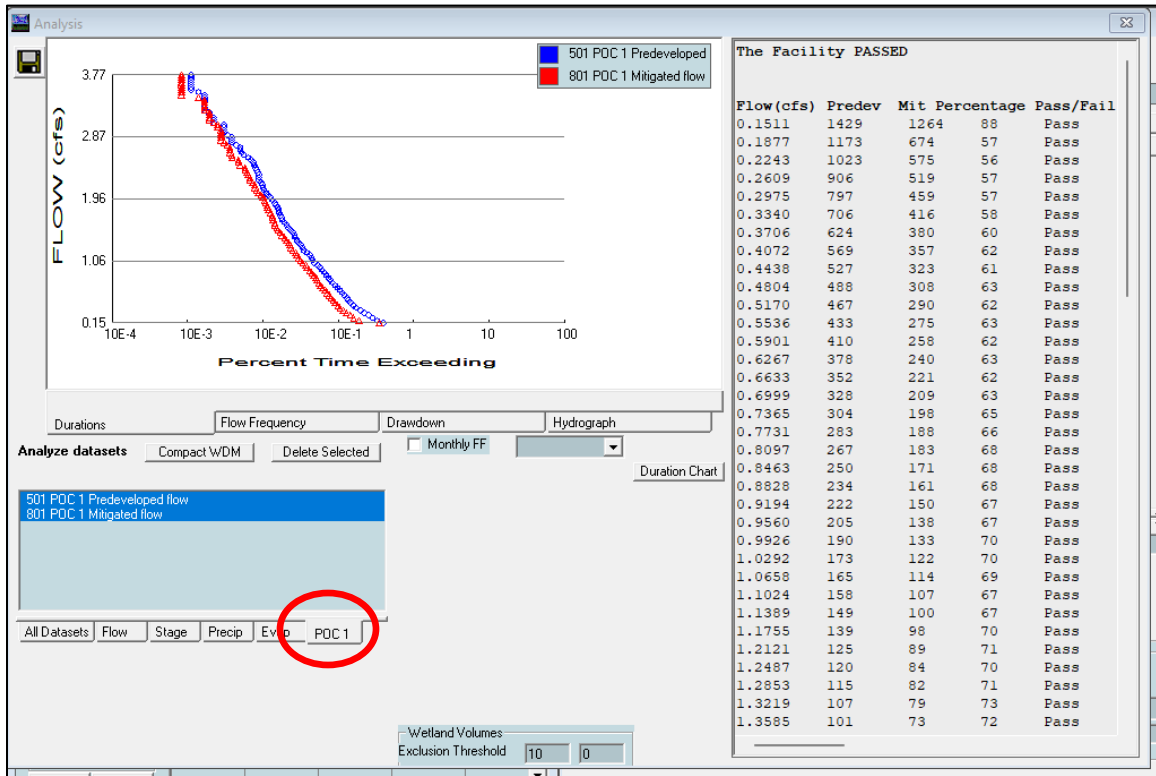

The Analysis tool bar button (third from the left) brings up the Analysis screen where the user can look at the results. Each time series dataset is listed in the Analyze Datasets box in the lower left corner. To review the flow duration analysis at the point of compliance select the POC 1 tab at the bottom and make sure that both the 501 POC 1 Pre-project flow and 801 POC 1 Developed flow are highlighted. Click the Run Analysis button if the flow duration analysis is not automatically computed.

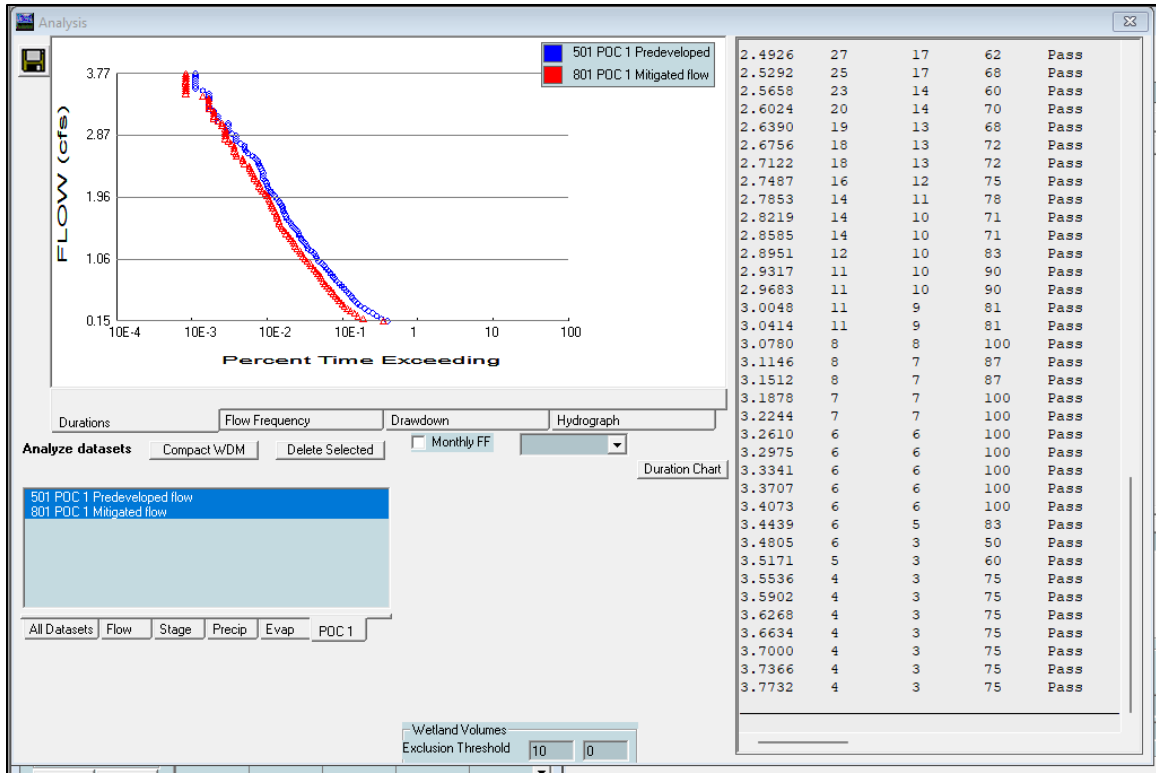


The flow duration plot for both Pre-project and Mitigated flows will be shown along with the specific flow values and number of times Pre-project and Mitigated flows exceeded those flow values. The Pass/Fail on the right indicates whether or not at that flow level the flow control standard criteria were met, and the pond passes at that flow level (from 10% of the 2-year flow to the 10-year). If not, a Fail is shown; one Fail fails the pond design.

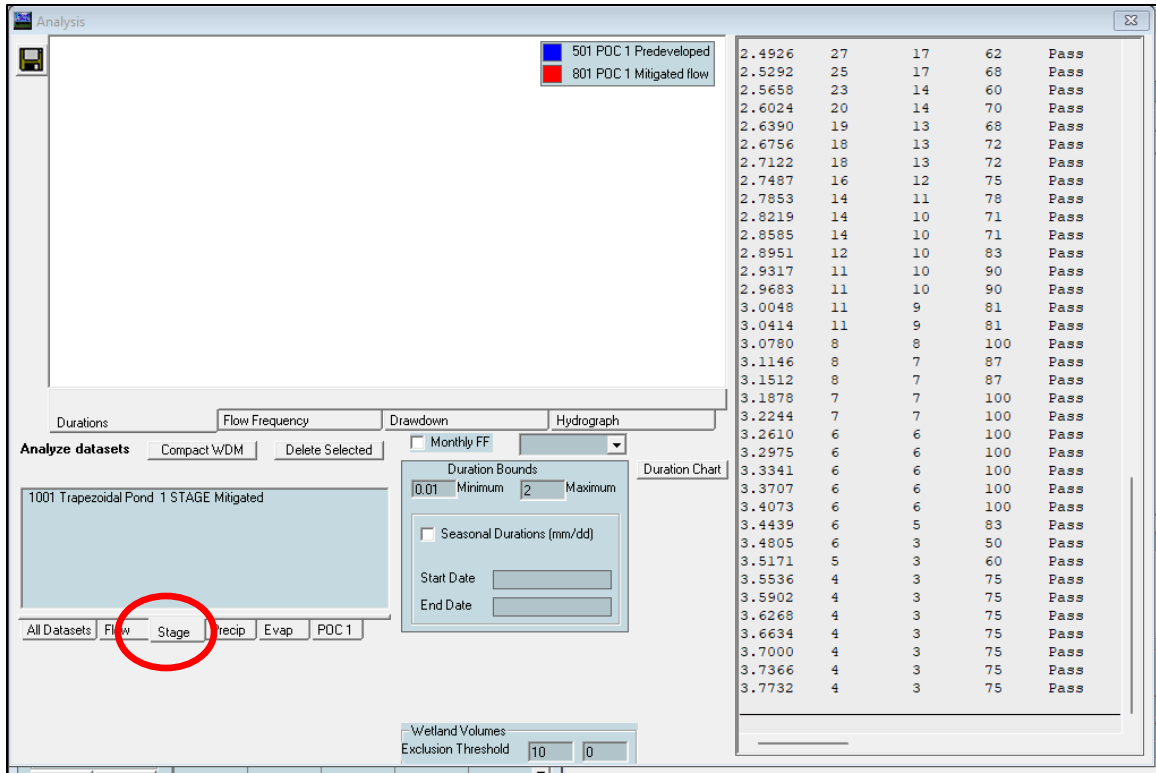

Pond drawdown/retention time is computed on the Analysis screen.

NOTE: This information is not required for basic sizing of the flow duration facility but can assist the user in minimizing risk of vector (mosquito) breeding problems. See page 139 for more descriptions of this BAHM2023 feature, and Appendix D for discussion and references for these requirements.

Click on the Stage tab at the bottom to get the Mitigated Pond stage time series.

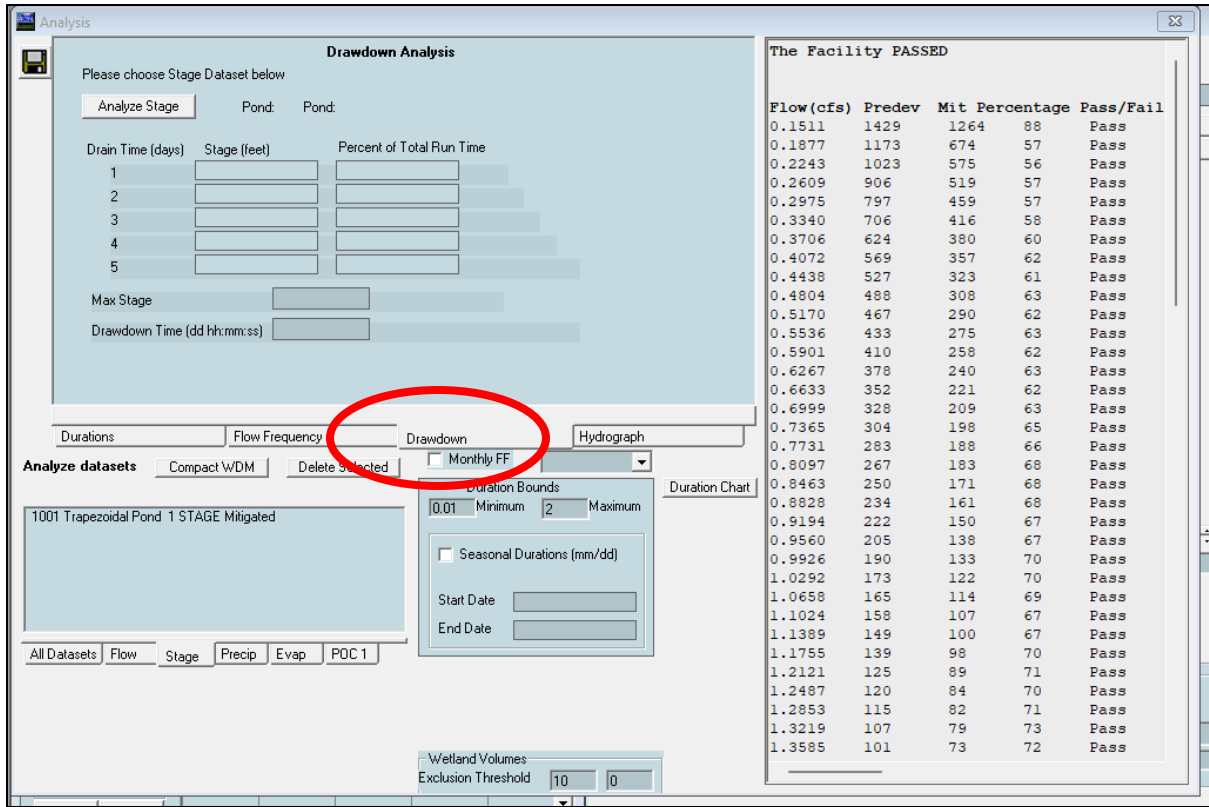

Click on the tab labeled Drawdown. This is where the pond drawdown/retention time results will be shown.

Drawdown Analysis

Select analysis for 1001 Trapezoidal Pond 1 STAGE Mitigated

Analyze Stage Pond: Pond:

Drain Time (days)	Stage (feet)	Percent of Total Run Time
1		
2		
3		
4		
5		

Max Stage:

Drawdown Time (dd hh:mm:ss):

Duration: Flow Frequency: Drawdown: Hydrograph:

Analyze datasets Compact WDM Delete Selected

1001 Trapezoidal Pond 1 STAGE Mitigated

All Datasets Flow Stage Precip Evap POC 1

Duration Bounds: Minimum Maximum

Seasonal Durations (mm/dd)

Start Date:


End Date:

Wetland Volumes
Exclusion Threshold:

The Facility PASSED

Flow (cfs)	Predev	Mit	Percentage	Pass/Fail
0.1511	1429	1264	88	Pass
0.1877	1173	674	57	Pass
0.2243	1023	575	56	Pass
0.2609	906	519	57	Pass
0.2975	797	459	57	Pass
0.3340	706	416	58	Pass
0.3706	624	380	60	Pass
0.4072	569	357	62	Pass
0.4438	527	323	61	Pass
0.4804	488	308	63	Pass
0.5170	467	290	62	Pass
0.5536	433	275	63	Pass
0.5901	410	258	62	Pass
0.6267	378	240	63	Pass
0.6633	352	221	62	Pass
0.6999	328	209	63	Pass
0.7365	304	198	65	Pass
0.7731	283	188	66	Pass
0.8097	267	183	68	Pass
0.8463	250	171	68	Pass
0.8828	234	161	68	Pass
0.9194	222	150	67	Pass
0.9560	205	138	67	Pass
0.9926	190	133	70	Pass
1.0292	173	122	70	Pass
1.0658	165	114	69	Pass
1.1024	158	107	67	Pass
1.1389	149	100	67	Pass
1.1755	139	98	70	Pass
1.2121	125	89	71	Pass
1.2487	120	84	70	Pass
1.2853	115	82	71	Pass
1.3219	107	79	73	Pass
1.3585	101	73	72	Pass

Select the pond you want to analyze for drawdown/retention time (in this example there is only one pond: Trapezoidal Pond 1) by clicking on the dataset and highlighting it.

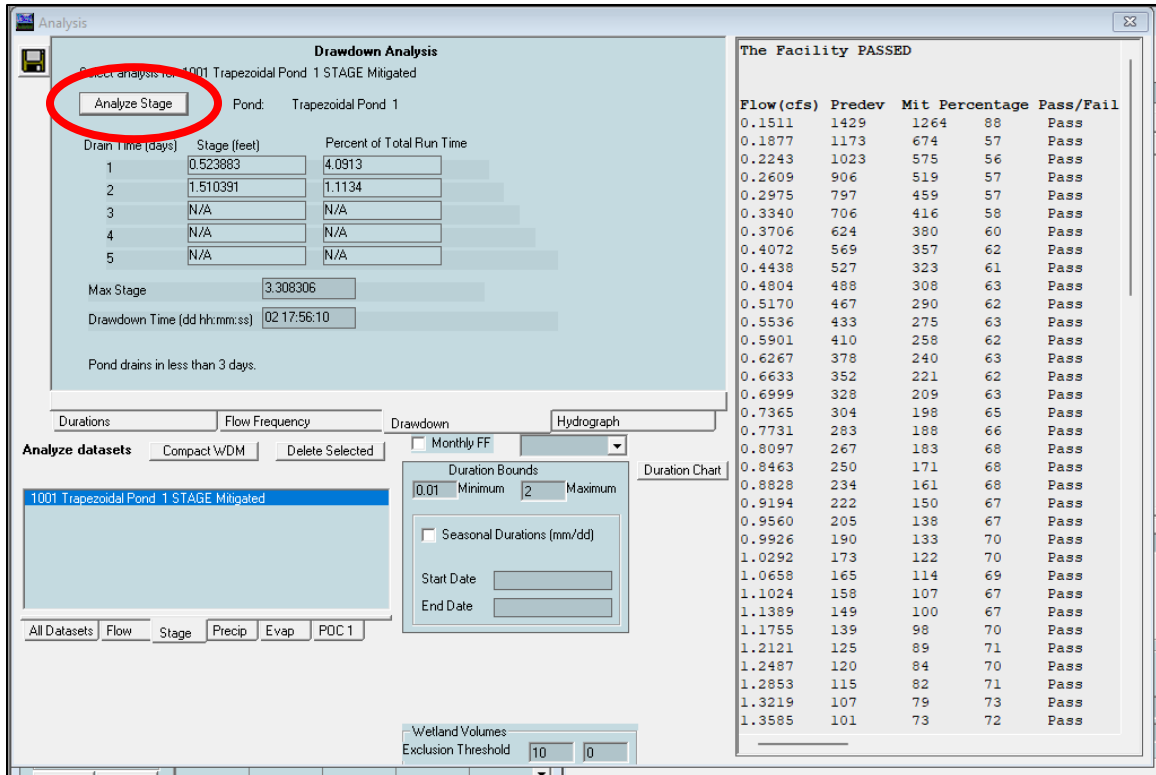


Click on the Analyze Stage button and the computed pond stages (pond water depths) are summarized and reported in terms of drain/retention time (in days).

For this example, a stage/depth of 0.52 feet occurred 4.09% of the time and took 1 day on average to drain (because of continuing inflows to the pond). The pond depth of 1.51 feet occurred 1.11% of the time and took 2 days on average to drain for the same reason. The maximum stage computed during the entire 35–50-year simulation period is 3.31 feet. This maximum stage has a drawdown time of 2 days, 17 hours, 56 minutes, 10 seconds.

Stages can have drain times in excess of 5 days. This can occur when a pond has a small bottom orifice. If this is not acceptable then the user needs to change the pond outlet configuration, manually run the Mitigated scenario, and repeat the analyze stage computations. A situation may occur where it is not possible to have both an acceptable pond drawdown/ retention time and meet the flow duration criteria.

NOTE: See Appendix D or the local municipal permitting agency for an overview of other requirements that may apply regarding drawdown time, and suggestions for addressing situations where it is not possible to meet all drawdown/retention time guidelines and also meet the flow duration criteria. The user manual assumes that the flow duration criteria take precedence unless the user is instructed otherwise by the local municipal permitting agency.

6. Produce report.

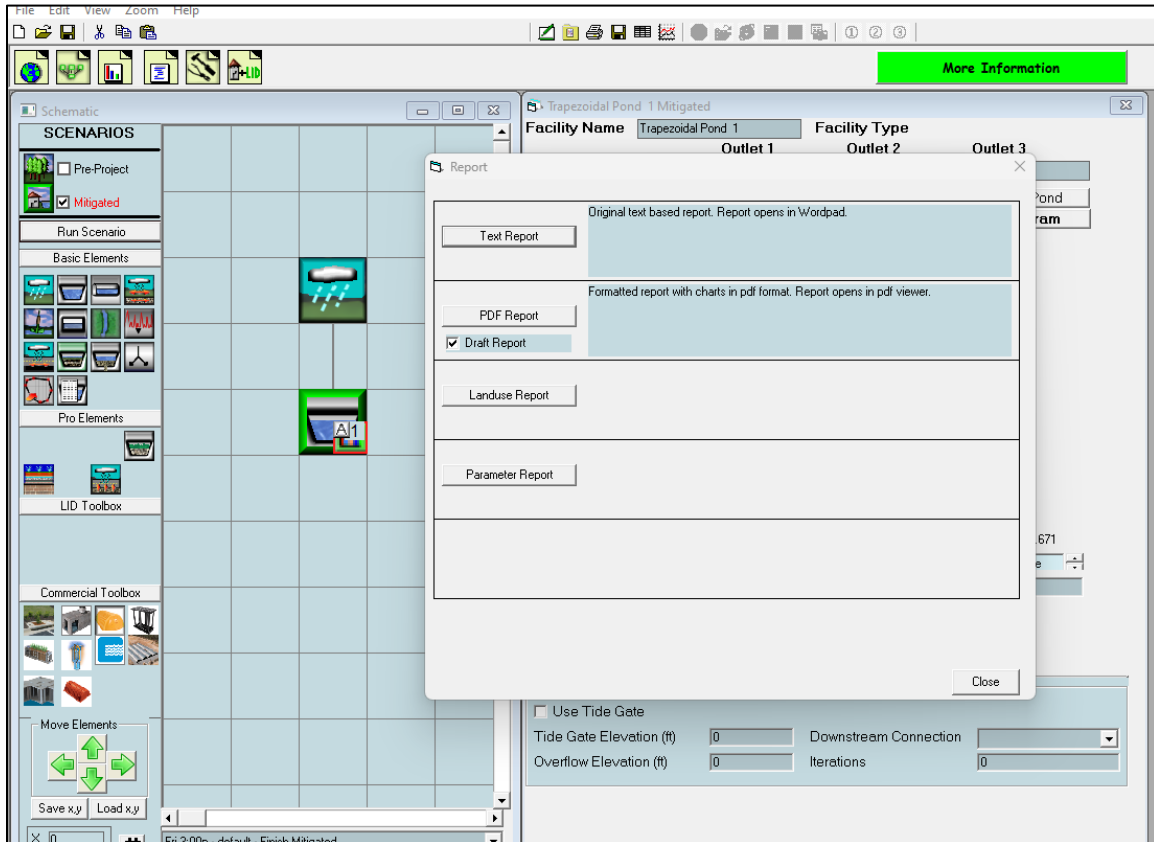

Click on the Reports tool bar button (fourth from the left) to generate a project report with all of the project information and results.

The project report can be generated as either a Microsoft Word file or a PDF file.

General Model Information

BAHM2023 Project Name: default
Site Name:
Site Address:
City:
Report Date: 4/28/2023
Gage: San Jose
Data Start: 1959/10/01
Data End: 2000/09/30
Timestep: Hourly
Precip Scale: 0.862
Version Date: 2023/04/26


POC Thresholds

Low Flow Threshold for POC1:	10 Percent of the 2 Year
High Flow Threshold for POC1:	10 Year


DRAFT

Scroll down the Report screen to see all of the results.

7. Save project.

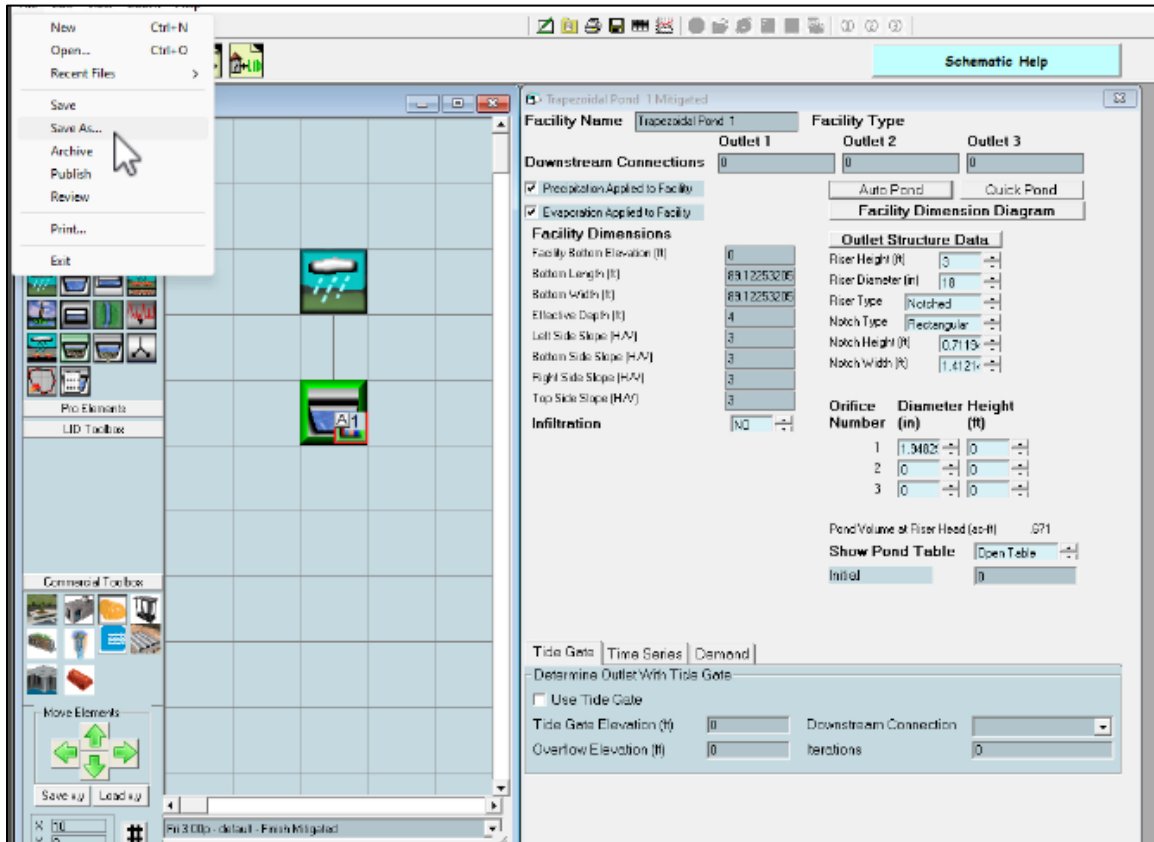


To save the project click on File in the upper left corner and select Save As.

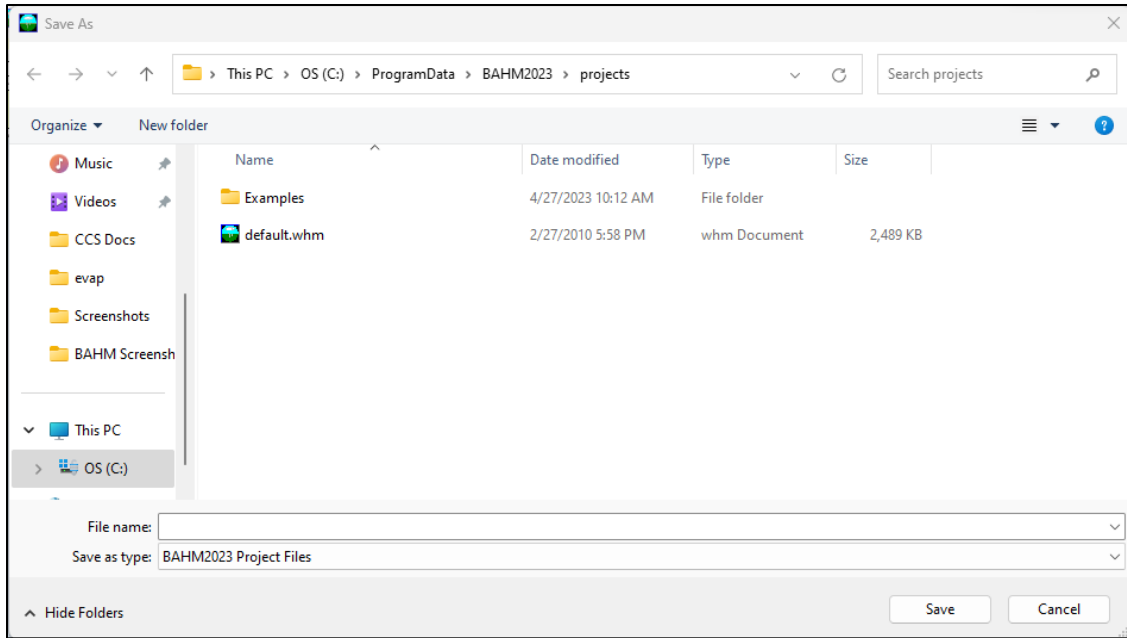

Select a file name and save the BAHM2023 project file. The user can exit BAHM2023 and later reload the project file with all of its information by going to File, Open.

8. Exit BAHM2023.

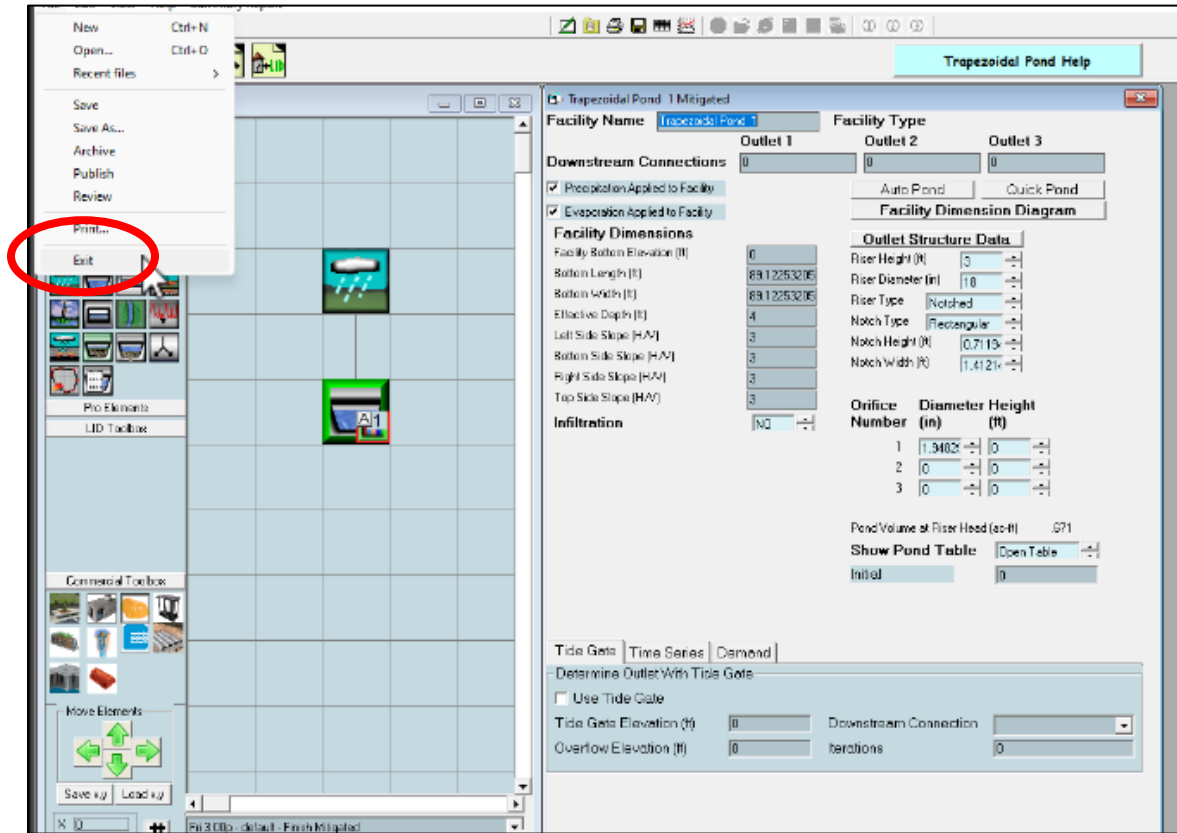

To exit BAHM2023 click on File in the upper left corner and select Exit. Or click on the X in the red box in the upper right-hand corner of the screen.

Learn more about Quick Start Modeling here:
www.clearcreeksolutions.info/bahm-course-home

MAIN SCREENS




BAHM2023 has six main screens. These main screens can be accessed through the buttons shown on the tool bar above or via the View menu.

The six main screens are:

- Map Information
- General Project Information
- Analysis
- Reports
- Tools
- LID (Low Impact Development) Analysis

Each is discussed in more detail in the following sections.

MAP INFORMATION SCREEN

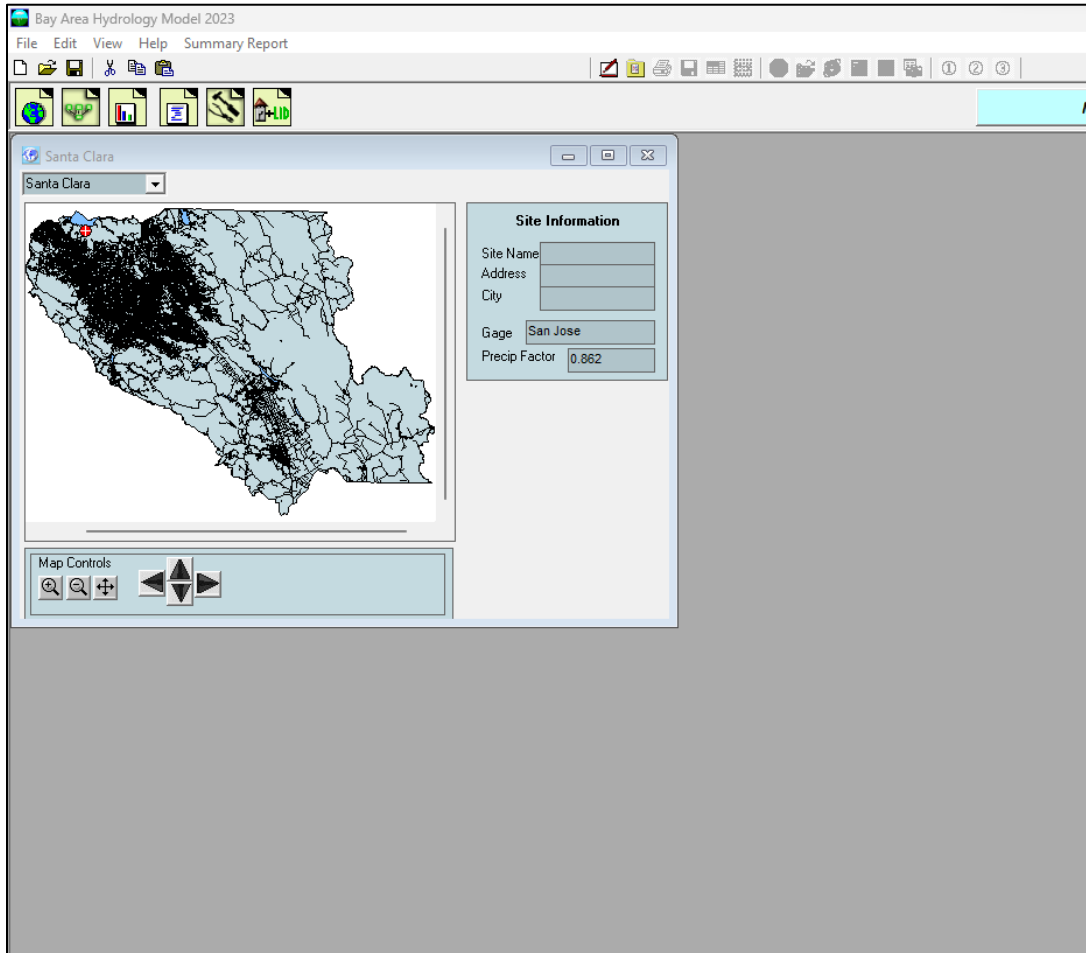

The Map Screen contains county information. The map is directly linked to the meteorological database that contains precipitation and evaporation data. The precipitation gage and precip factor are shown to the right of the map. They change depending on the project site location. See Appendix F for more information on the precipitation gages used and how the precipitation data are scaled to the location.


The county selection can be changed by clicking on the pulldown menu above the map and selecting one of the four Bay Area counties.

The user can provide site information (optional). The site name and address will help to identify the project on the Report screen and in the printed report provided to the local municipal permitting agency. Adding the site address does not replace selecting the project location on the map screen.

The user locates the project site on the map screen by using the mouse and left clicking at the project site location. Right clicking on the map re-centers the view. The + and –

buttons zoom in and out, respectively. The crosshair button zooms out to the full county view. The arrow keys scroll the map view.

GENERAL PROJECT INFORMATION SCREEN

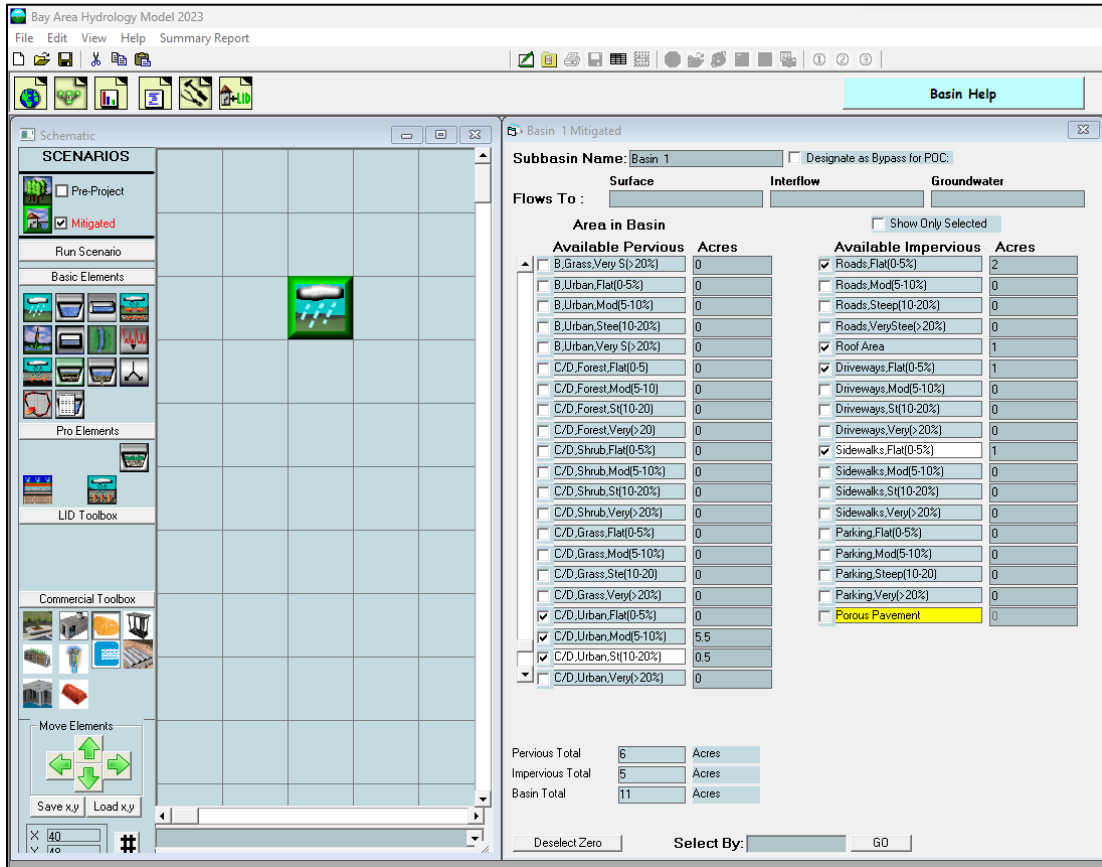


The project screen contains all of the information about the project site for the two land use scenarios: Pre-project land use conditions and the Mitigated (post-project) land use conditions. To change from one scenario to another check the box in front of the scenario name in the upper left corner of the screen.

Pre-project is defined as the existing conditions prior to the proposed land use development. Runoff from the Pre-project scenario is used as the target for the Mitigated scenario compliance. The model will accept any land use for this scenario.

Mitigated is defined as the developed land use with mitigation measures (as selected by the user). The Mitigated scenario is used for sizing hydromodification control facilities. The runoff from the Mitigated scenario is compared with the Pre-project scenario runoff to determine compliance with flow duration criteria.

Below the scenario boxes are the Elements. Each element represents a specific feature (basin, pond, etc.) and is described in more detail in the following section.

SCHEMATIC EDITOR

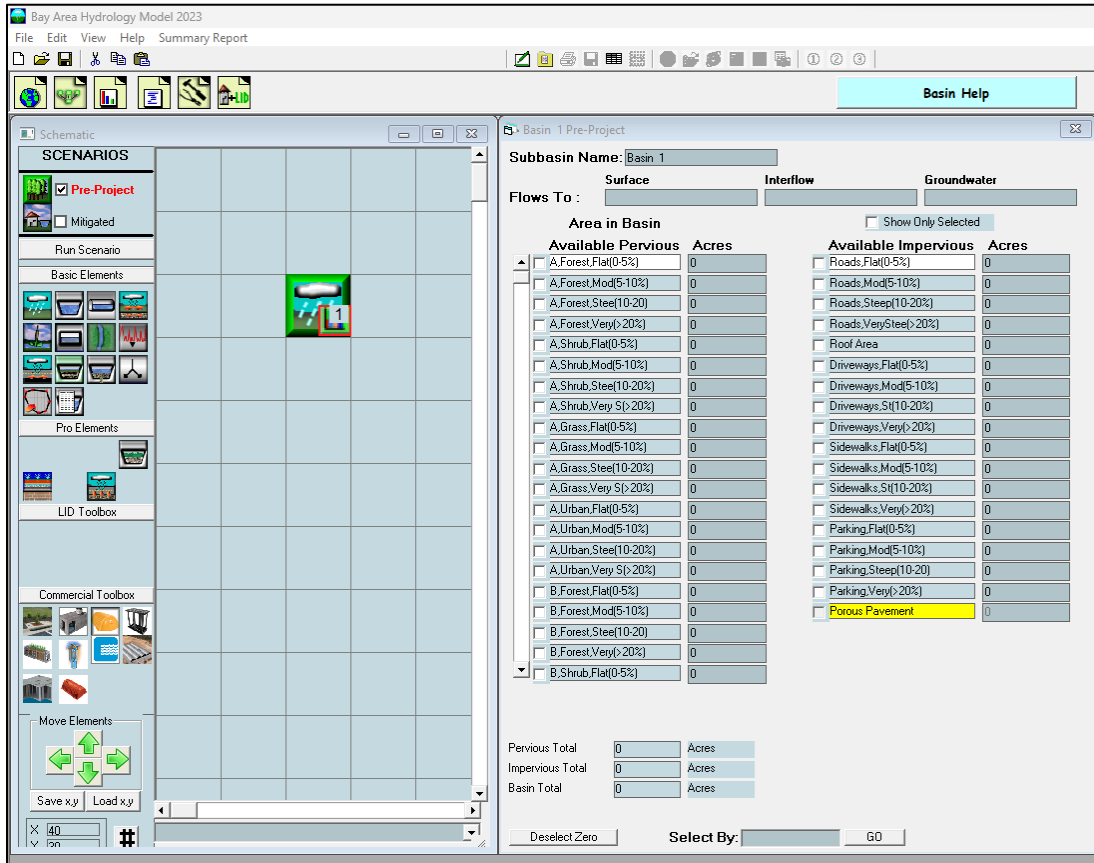

The project screen also contains the Schematic Editor. The Schematic Editor is the grid to the right of the elements. This grid is where each element is placed and linked together. The grid, using the scroll bars on the left and bottom, expands as large as needed to contain all of the elements for the project.

All movement on the grid must be from the top of the grid down.

The space to the right of the grid will contain the appropriate element information.

To select and place an element on the grid, first left click on the specific element in the Elements menu and then left click on the selected grid square. The selected element will appear in the grid square.

The entire grid can be moved up, down, left, or right using the Move Elements arrow buttons.

The grid coordinates from one project can be saved (Save x,y) and used for new projects (Load x,y).

The following discussion of the Schematic Editor is divided into Standard Elements, Pro Elements and LID Toolbox.

Standard Elements include: Basin, Trapezoidal Pond, Vault, Tank, Irregular Pond, Gravel Trench Bed, Sand Filter, Channel, Flow Splitter, Time Series, SSD Table, and High Groundwater/Wetland element, Lateral Flow Soil Basin (Pervious), Lateral Flow Impervious Area (Impervious).

Pro Elements included (included in all versions of BAHM2023): Bioretention, Permeable Pavement, and Green Roof. In previous versions of the software, these elements were available as part of a “Pro” version and were added after the basic elements. In BAHM2023, all users have access to these elements.

LID Toolbox: In-Ground Planter, In-Ground Infiltration Planter Box, Flow-Through Planter Box, Infiltration Basin, Infiltration Trench, and Dry Well.


Learn more about the BAHM Schematic here:
www.clearcreeksolutions.info/bahm-course-home

STANDARD ELEMENTS

The following pages contain information about these standard elements:

- Basin
- Trapezoidal Pond
- Vault
- Tank
- Irregular Pond
- Gravel Trench Bed
- Sand Filter
- Channel
- Flow Splitter
- Time Series
- SSD Table
- High Groundwater/Wetland
- Lateral Flow Soil Basin (Pervious)
- Lateral Flow Impervious Area (Impervious)

BASIN ELEMENT

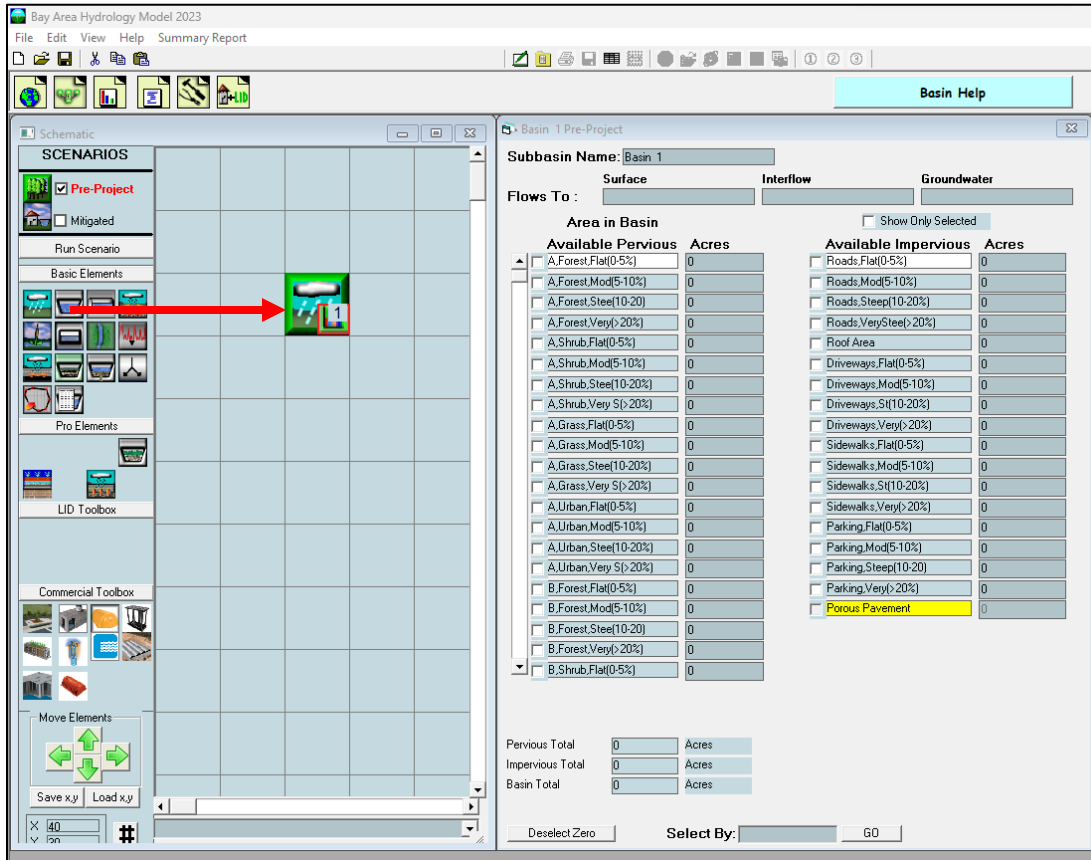

The Basin element represents a drainage area that can have any combination of soils, vegetation, and land uses. A basin produces three types of runoff: (1) surface runoff, (2) interflow, and (3) groundwater.

Surface runoff is defined as the overland flow that quickly reaches a conveyance system. Surface runoff mainly comes from impervious surfaces.

Interflow is shallow, subsurface flow produced by pervious land categories and varies based on soil characteristics and how these characteristics are altered by land development practices.

Groundwater is the subsurface flow that typically does not enter a stormwater conveyance system but provides base flow directly to streams and rivers.

The user can specify where each of these three types of runoff should be directed. The default setting is for the surface runoff and interflow to go to the stormwater facility; groundwater should not be connected unless there is observed base flow occurring in the drainage basin.

Table 1 shows the different pervious land types represented in the Basin element.

Table 1. BAHM2023 Pervious Land Types

PERLND No.	Soil	Vegetation/Surface	Slope
1	A	Forest	Flat(0-5%)
2	A	Forest	Moderate(5-10%)
3	A	Forest	Steep(10-20%)
4	A	Forest	Very Steep(>20%)
5	A	Shrub	Flat(0-5%)
6	A	Shrub	Moderate(5-10%)
7	A	Shrub	Steep(10-20%)
8	A	Shrub	Very Steep(>20%)
9	A	Grass	Flat(0-5%)
10	A	Grass	Moderate(5-10%)
11	A	Grass	Steep(10-20%)
12	A	Grass	Very Steep(>20%)
13	A	Urban	Flat(0-5%)
14	A	Urban	Moderate(5-10%)
15	A	Urban	Steep(10-20%)
16	A	Urban	Very Steep(>20%)
17	B	Forest	Flat(0-5%)
18	B	Forest	Moderate(5-10%)
19	B	Forest	Steep(10-20%)
20	B	Forest	Very Steep(>20%)
21	B	Shrub	Flat(0-5%)
22	B	Shrub	Moderate(5-10%)
23	B	Shrub	Steep(10-20%)
24	B	Shrub	Very Steep(>20%)
25	B	Grass	Flat(0-5%)
26	B	Grass	Moderate(5-10%)
27	B	Grass	Steep(10-20%)
28	B	Grass	Very Steep(>20%)
29	B	Urban	Flat(0-5%)
30	B	Urban	Moderate(5-10%)
31	B	Urban	Steep(10-20%)
32	B	Urban	Very Steep(>20%)
33	C/D	Forest	Flat(0-5%)
34	C/D	Forest	Moderate(5-10%)
35	C/D	Forest	Steep(10-20%)
36	C/D	Forest	Very Steep(>20%)
37	C/D	Shrub	Flat(0-5%)
38	C/D	Shrub	Moderate(5-10%)
39	C/D	Shrub	Steep(10-20%)
40	C/D	Shrub	Very Steep(>20%)
41	C/D	Grass	Flat(0-5%)

PERLND No.	Soil	Vegetation/Surface	Slope
42	C/D	Grass	Moderate(5-10%)
43	C/D	Grass	Steep(10-20%)
44	C/D	Grass	Very Steep(>20%)
45	C/D	Urban	Flat(0-5%)
46	C/D	Urban	Moderate(5-10%)
47	C/D	Urban	Steep(10-20%)
48	C/D	Urban	Very Steep(>20%)

The user does not need to know or keep track of the HSPF PERLND number. That number is used only for internal tracking purposes in the HSPF UCI file created by BAHM2023.

The user inputs the number of acres of appropriate basin land use information. Pervious land use information is in the form of soil, vegetation, and land slope. For example, “A, Grass, Flat” means NRCS soil type A, non-turf grassland vegetation, and flat (0-5%) land slope.

There are three basic soil types: A (well infiltrating soils), B (moderate infiltrating soils), and C/D (poor infiltrating soils).

There are four basic vegetation categories: forest, native shrub rural vegetation, non-turf grasslands, and urban landscaped vegetation.

Natural vegetation has been divided into forest, shrub, and non-turf grass and refers to the natural (non-planted) vegetation. In contrast, the developed landscape will consist of urban vegetation (lawns, flowers, planted shrubs and trees). Urban vegetation is irrigated in the model using a pre-input irrigation time series, which is a calibrated irrigation time series that represents irrigation on landscaped areas.

Land slope is divided into flat (0-5%), moderate (5-10%), steep (10-20%), and very steep (>20%) land slopes.

HSPF parameter values in BAHM2023 have been adjusted for the different soil, vegetation, and land slope categories. BAHM2023 HSPF soil parameter values take into account the hydrologic effects of land development activities that result from soil compaction when “Urban” is specified.

Impervious areas are divided into five types with four different slopes (see Table 2). The five types are: roads, roofs, driveways, sidewalks, and parking. The slope categories are the same as for the pervious land use (flat, moderate, steep, and very steep).

Table 2. BAHM2023 Impervious Land Types

IMPLND No.	Surface	Slope
1	Roads	Flat (0-5%)
2	Roads	Mod (5-10%)
3	Roads	Steep (10-20%)
4	Roads	Very Steep (>20%)
5	Roof	Flat (0-5%)
6	Driveways	Flat (0-5%)
7	Driveways	Mod (5-10%)
8	Driveways	Steep (10-20%)
9	Driveways	Very Steep (>20%)
10	Sidewalks	Flat (0-5%)
11	Sidewalks	Mod (5-10%)
12	Sidewalks	Steep (10-20%)
13	Sidewalks	Very Steep (>20%)
14	Parking	Flat (0-5%)
15	Parking	Mod (5-10%)
16	Parking	Steep (10-20)
17	Parking	Very Steep (>20%)
18	Porous Pavement	N/A

The user does not need to know or keep track of the HSPF IMPLND number. That number is used only for internal tracking purposes in the HSPF UCI file created by BAHM2023.


There are five different impervious area types available and four different slopes. Roads, Driveways, Sidewalks and Parking all behave exactly the same way; they are listed as separate types for organizational purposes only. This allows the user to categorize the impervious area by type. Each of these four types also has four slope options available. Runoff from each of the impervious type and slope combinations is exactly the same. For example, runoff from Roads Flat (0-5%) is the same as runoff from Driveways Flat (0-5%).

Roof area is the same as the other four types, Roads, Driveways, Sidewalks and Parking but Roofs only has one slope available (Flat). Impervious areas of the same slope type are calculated the same in BAHM 2023.

Porous Pavement is different from the impervious area options. This is not an option that should be selected from within the basin. Porous pavement is part of the porous pavement element. Each time a porous pavement element is added to the model a duplicate of the porous pavement impervious surface is added internally.


Learn more about the BAHM Schematic here:
www.clearcreeksolutions.info/bahm-course-home

TRAPEZOIDAL POND ELEMENT

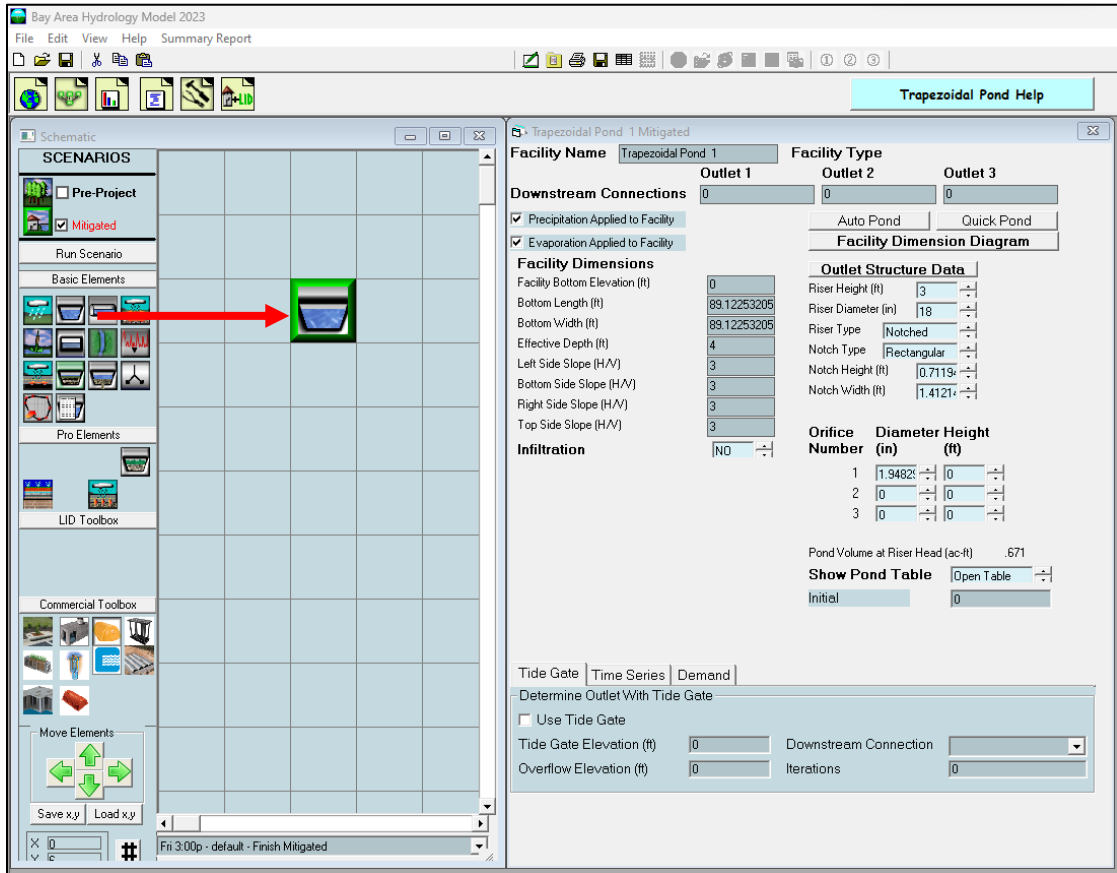

In BAHM2023 there is an individual pond element for each type of pond and stormwater control facility. The pond element shown above is for a trapezoidal pond. This is the most common type of stormwater pond.

A trapezoidal pond has dimensions (bottom length and width, depth, and side slopes) and an outlet structure consisting of a riser and one or more orifices to control the release of stormwater from the pond. A trapezoidal pond includes the option to infiltrate runoff, if the soils are appropriate and there is sufficient depth to the underlying groundwater table.

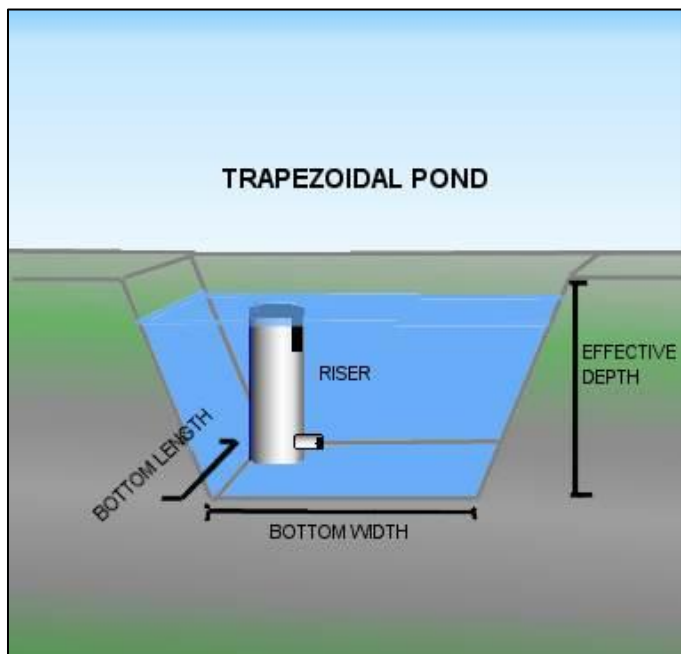

The user has the option to specify that different outlets be directed to different downstream destinations, although usually all of the outlets go to a single downstream location.

Auto Pond will automatically size a trapezoidal pond to meet the required flow duration criteria. Auto Pond is available only in the Mitigated scenario.

Quick Pond can be used to instantly add pond dimensions and an outlet configuration without checking the pond for compliancy with flow duration criteria. Quick Pond is sometimes used to quickly create a scenario and check the model linkages prior to sizing the pond. Multiple clicks on the Quick Pond button incrementally increase the pond size.

The user can change the default name “Trapezoidal Pond 1” to another more appropriate name, if desired.

Precipitation and evaporation are automatically applied to the pond unless the pond is covered.

The pond bottom elevation can be set to an elevation other than zero if the user wants to use actual elevations. All pond stage values are relative to the bottom elevation. Negative bottom elevations are not allowed.

The pond effective depth is the pond height (including freeboard) above the pond bottom. It is not the actual elevation of the top of the pond.

Pond side slopes are in terms of horizontal distance over vertical. A standard 3:1 (H/V) side slope would be given a value of 3. A vertical side slope has a value of 0.

The pond bottom is assumed to be flat.

The pond outlet structure consists of a riser and zero to three orifices. The riser has a height (typically one foot less than the effective depth) and a diameter. The riser can have either a flat top or a weir notch cut into the side of the top of the riser. The notch can be either rectangular, V-shaped, or a Sutro weir. More information on the riser weir shapes and orifices is provided later in this manual.

After the pond is given dimensions and outlet information the user can view the resulting stage-storage-discharge table by clicking on the “Open Table” arrow in the lower right corner of the pond information screen. This table hydraulically defines the pond’s characteristics.

The user can use either Auto Pond to size a pond or can manually size a pond. Use the following steps for manual sizing a pond using an outlet configuration with one orifice and a riser with rectangular notch (this is usually the most efficient design):

1. Input the pond bottom length, width, side slopes, and effective depth (height of riser plus freeboard).
2. Input a bottom orifice diameter that allows a discharge equal to 10% of the 2-year Pre-project flow for a stage equal to 2/3rds the height of the riser. This discharge can be checked by reviewing the pond's stage-storage-discharge table.
3. Input a riser rectangular notch height equal to 1/3 of the height of the riser. Initially set the riser notch width to 0.1 feet.
4. Run Pre-project and Mitigated scenarios.
5. Go to Analysis screen and check flow duration results.
6. If pond passes flow duration criteria then decrease pond dimensions.
7. If pond fails flow duration criteria then change (in order) bottom orifice diameter, riser notch width, pond dimensions.
8. Iterate until there is a good match between Pre-project and Mitigated flow duration curves or fatigue sets in.

Pond input information:

Bottom Length (ft): Pond bottom length.

Bottom Width (ft): Pond bottom width.

Effective Depth (ft): Pond height from pond bottom to top of riser plus at least 0.5 feet extra.

Left Side Slope (H/V): ratio of horizontal distance to vertical; 0 (zero) for vertical pond sides.

Bottom Side Slope (H/V): ratio of horizontal distance to vertical; 0 (zero) for vertical pond sides.

Right Side Slope (H/V): ratio of horizontal distance to vertical; 0 (zero) for vertical pond sides.

Top Side Slope (H/V): ratio of horizontal distance to vertical; 0 (zero) for vertical pond sides.

Riser Height (ft): Height of overflow pipe above pond bottom.

Riser Diameter (in): Pond overflow pipe diameter.

Riser Type (options): Flat or Notched

Notch Type: Rectangular, V-Notch, or Sutro.

For a rectangular notch:

Notch Height (feet): distance from the top of the weir to the bottom of the notch.

Notch Width (feet): width of notch; cannot be larger than the riser circumference.

For more information on riser notch options and orifices see discussion in OUTLET STRUCTURE CONFIGURATIONS section.

Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

Infiltration Reduction Factor: 1/Native soil infiltration rate safety factor (see page 123).

Use Wetted Surface Area (sidewalls): Yes, if infiltration through the pond side slopes is allowed.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

A pond receives precipitation on and evaporation from the pond surface. The Precipitation Applied to Facility and Evaporation Applied to Facility boxes should be checked.

NOTE: The following detention pond section diagram shows the general configuration used in designing a pond and its outlet structure. This diagram is from the Washington State Department of Ecology's 2005 Stormwater Management Manual for Western Washington. Consult with your local municipal permitting agency on specific design requirements for your project site.


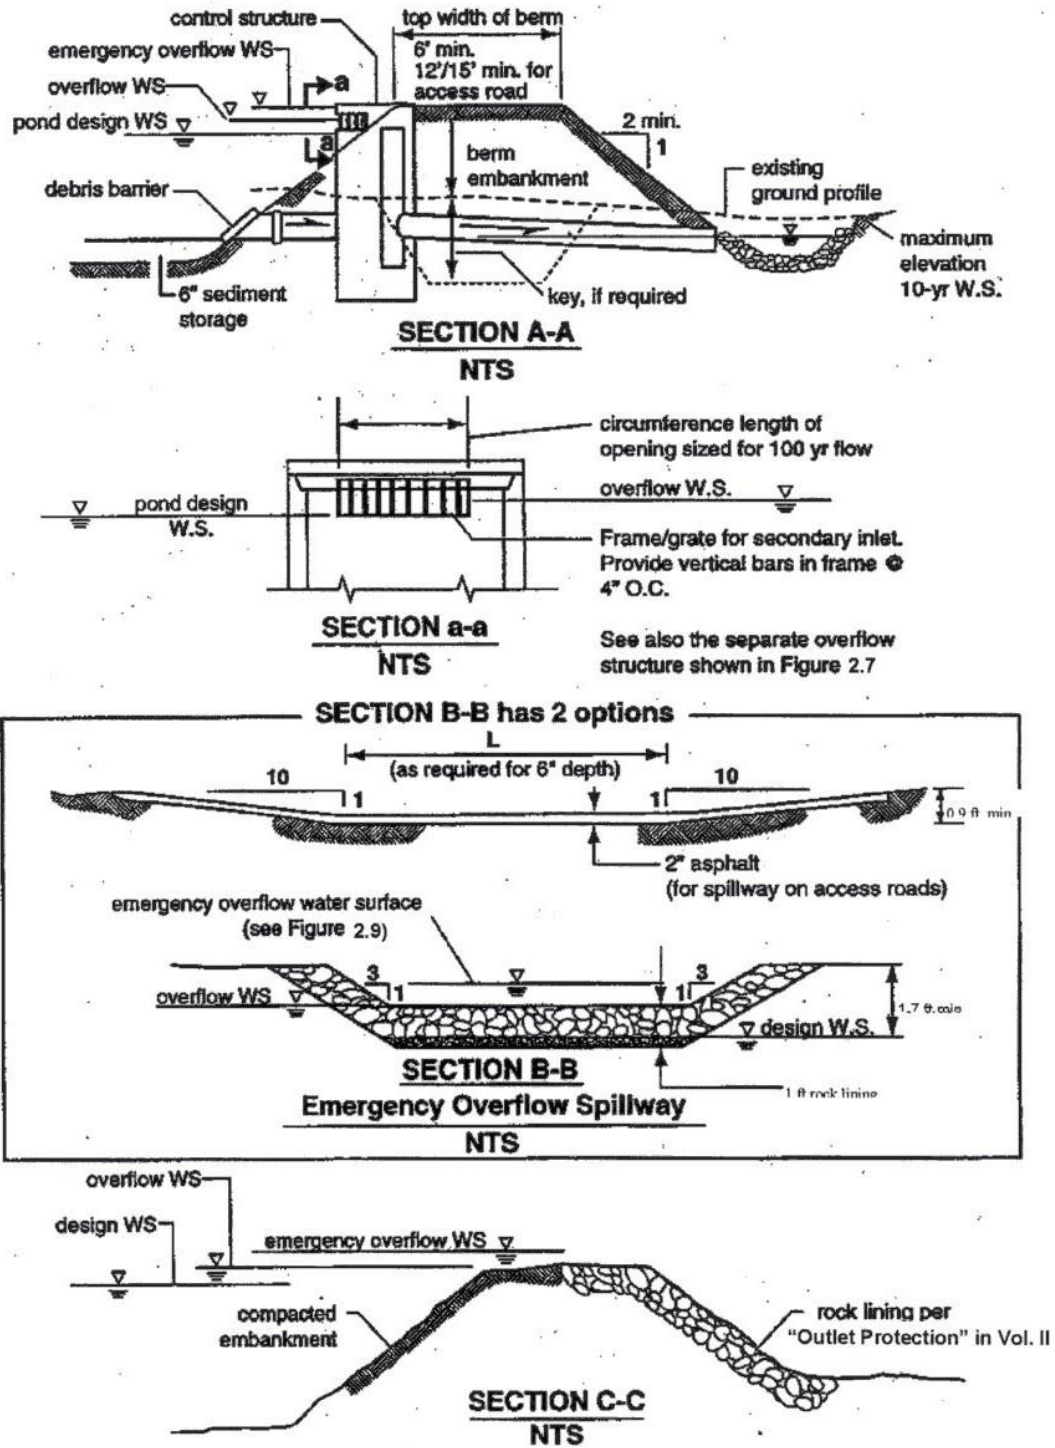


Figure 3.10 Typical Detention Pond Sections

VAULT ELEMENT

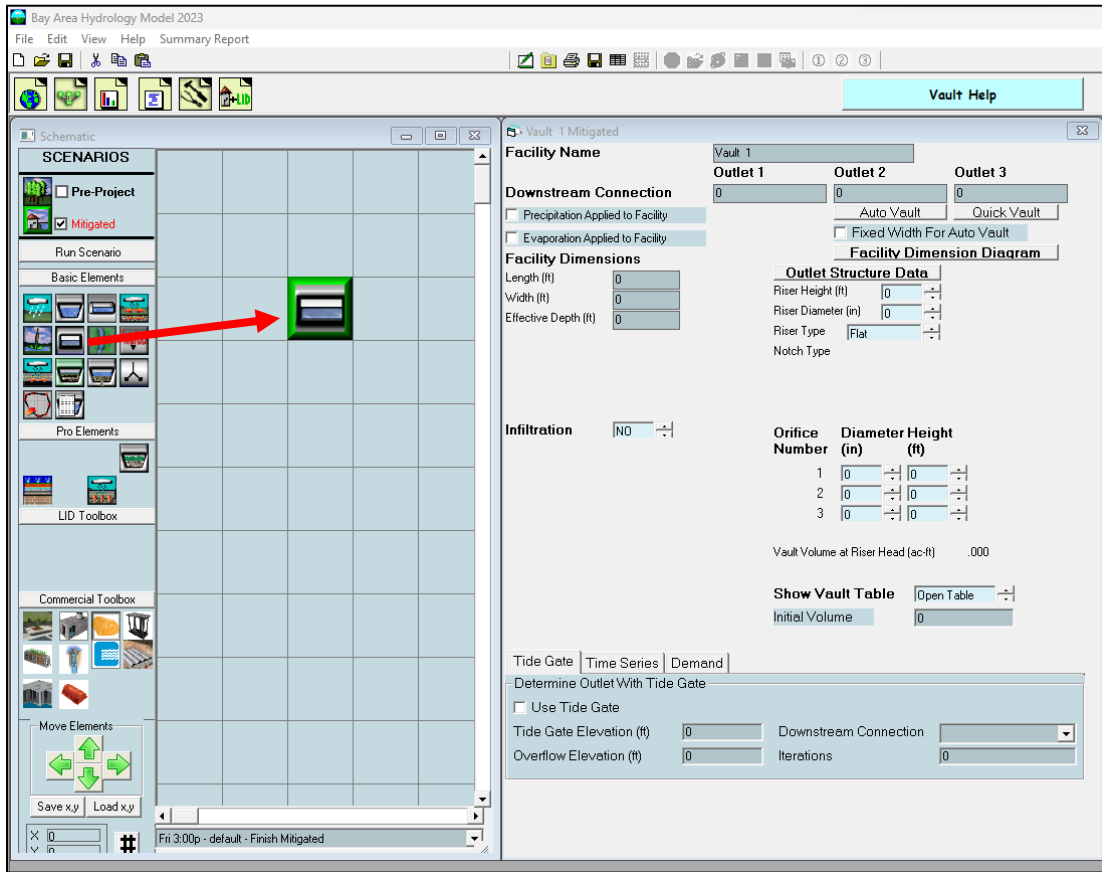

The storage vault has all of the same characteristics of the trapezoidal pond, except that the user does not specify the side slopes (by definition they are zero).

AutoVault and Quick Vault work the same way as Auto Pond and Quick Pond. Go to page 46 to find information on how to manually size a vault or other HM facility.

Vault input information:

Bottom Length (ft): Vault bottom length.

Bottom Width (ft): Vault bottom width.


Effective Depth (ft): Vault height from vault bottom to top of riser plus freeboard (at least 0.5 feet extra).

Riser Height (ft): Height of overflow pipe above vault bottom.

Riser Diameter (in): Vault overflow pipe diameter.

Riser Type (options): Flat or Notched

Notch Type: Rectangular, V-Notch, or Sutor.

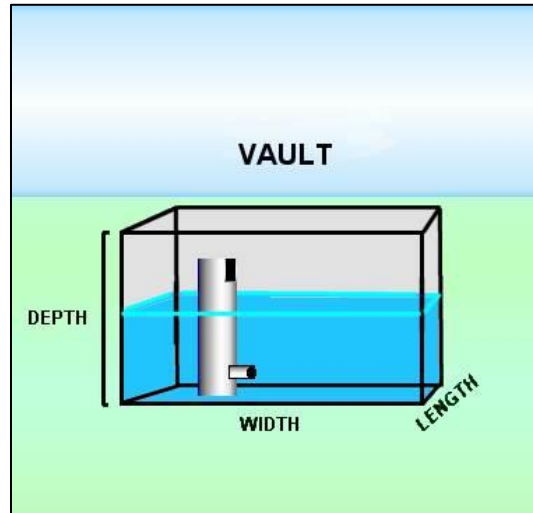

For a rectangular notch:

Notch Height (feet): distance from the top of the weir to the bottom of the notch.

Notch Width (feet): width of notch; cannot be larger than the riser circumference.

For more information on riser notch options and orifices see discussion in OUTLET STRUCTURE CONFIGURATIONS section.

Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

Infiltration Reduction Factor: $1/\text{Native soil infiltration rate safety factor}$ (see page 123).

Use Wetted Surface Area (sidewalls): Yes, if infiltration through the vault sides is allowed.


If infiltration is used, then the user should consult the Infiltration discussion on page 123.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

A vault is usually covered and does not receive precipitation on and evaporation from the vault surface. The Precipitation Applied to Facility and Evaporation Applied to Facility boxes should not be checked.

Learn more about the BAHM Schematic here:
www.clearcreeksolutions.info/bahm-course-home

TANK ELEMENT

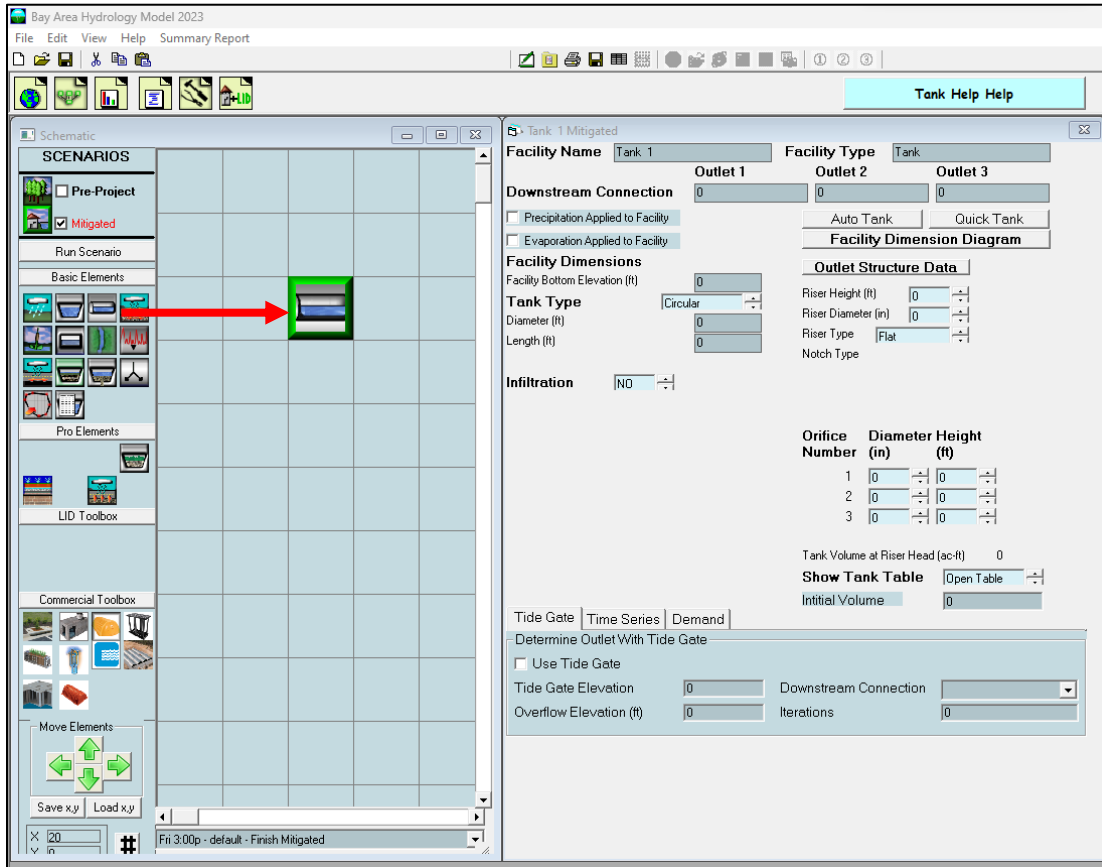

A storage tank is a cylinder placed on its side. The user specifies the tank’s diameter and length.

Auto Tank and Quick Tank work the same way as Auto Pond and Quick Pond.

Auto Tank is only available in the Mitigated scenario.

There is a Quick Tank option that creates a tank but does not check for compliance with the flow duration criteria.

Tank input information:

Tank Type: Circular or Arched

For Circular:


Diameter (ft): Tank diameter.

Length (ft): Tank length.

For Arched:

Height (ft): Tank height.

Width (ft): Tank width (at widest point).

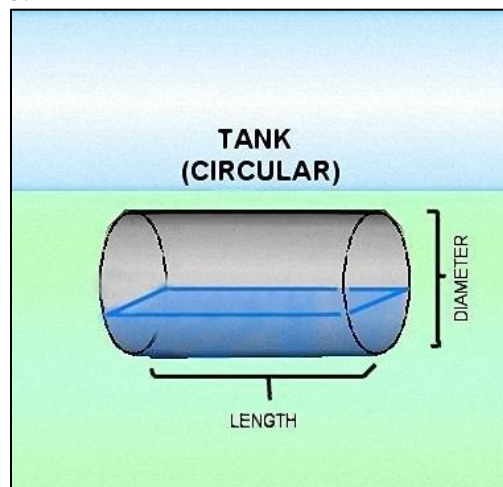

Length (ft): Tank length.

Riser Height (ft): Height of overflow pipe above tank bottom; must be less than tank diameter or height.

Riser Diameter (in): Tank overflow pipe diameter.

Riser Type (options): Flat or Notched


Notch Type: Rectangular, V-Notch, or Sutro.

For a rectangular notch:

Notch Height (feet): distance from the top of the weir to the bottom of the notch.

Notch Width (feet): width of notch; cannot be larger than the riser circumference.

For more information on riser notch options and orifices see discussion in OUTLET STRUCTURE CONFIGURATIONS section.

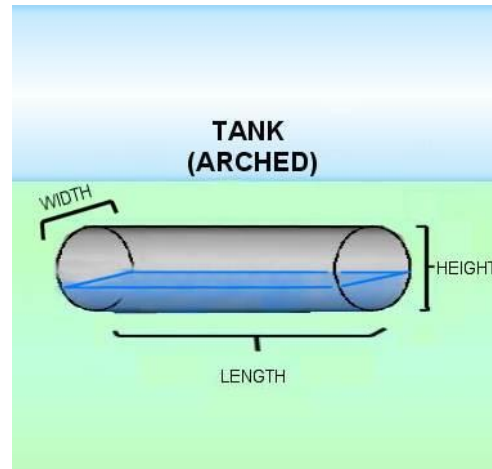

Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

Infiltration Reduction Factor: $1/\text{Native soil infiltration rate safety factor}$ (see page 123).

Use Wetted Surface Area (sidewalls): Yes, if infiltration through the tank sides is allowed.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

A tank is covered and does not receive precipitation on and evaporation from the tank surface. The Precipitation Applied to Facility and Evaporation Applied to Facility boxes should not be checked.

The tank element can be either cylindrical or arched. The tank element has dimensions (diameter and length and width or an arched tank) and an outlet structure consisting of a riser and one or more orifices to control the release of stormwater from the tank. The tank element includes the option to infiltrate runoff, if the soils are appropriate and there is sufficient depth to the underlying groundwater table.

When modeling a tank with a sloped bottom, follow the directions below.

The program determines the performance of the tank based on the assumption that the tank has zero bottom slope.

There are three factors that can impact this assumption.


- 1) The slope of the tank.
- 2) The length of the tank.
- 3) The diameter of the tank.

Slope can impact the actual storage of the tank if the slope to length and diameter ratio is high enough. For example, a 200-foot-long, 2-foot diameter tank with a bottom slope of 1% can lose a significant portion of the available storage at the upstream end of the tank. A water depth of 2 feet at the downstream end yields a depth of 0 at the upstream end. This reduces the overall storage capacity of the tank significantly. Alternatively, a 200-foot-long, 6-foot diameter tank with a bottom slope of 1% loses only a small amount of storage. A downstream depth of 6 feet yields a depth of 4 feet at the upstream end.

When using the tank for storage it is best to consider setting up a grid of interconnected storage tanks that are relatively short. If you need a 1000-foot, 4-foot diameter tank, it would be best to set up 10 rows of 100-foot-long pipe. This would reduce the impact of slope on the overall storage.

Learn more about the BAHM Schematic here:
www.clearcreeksolutions.info/bahm-course-home

IRREGULAR POND ELEMENT

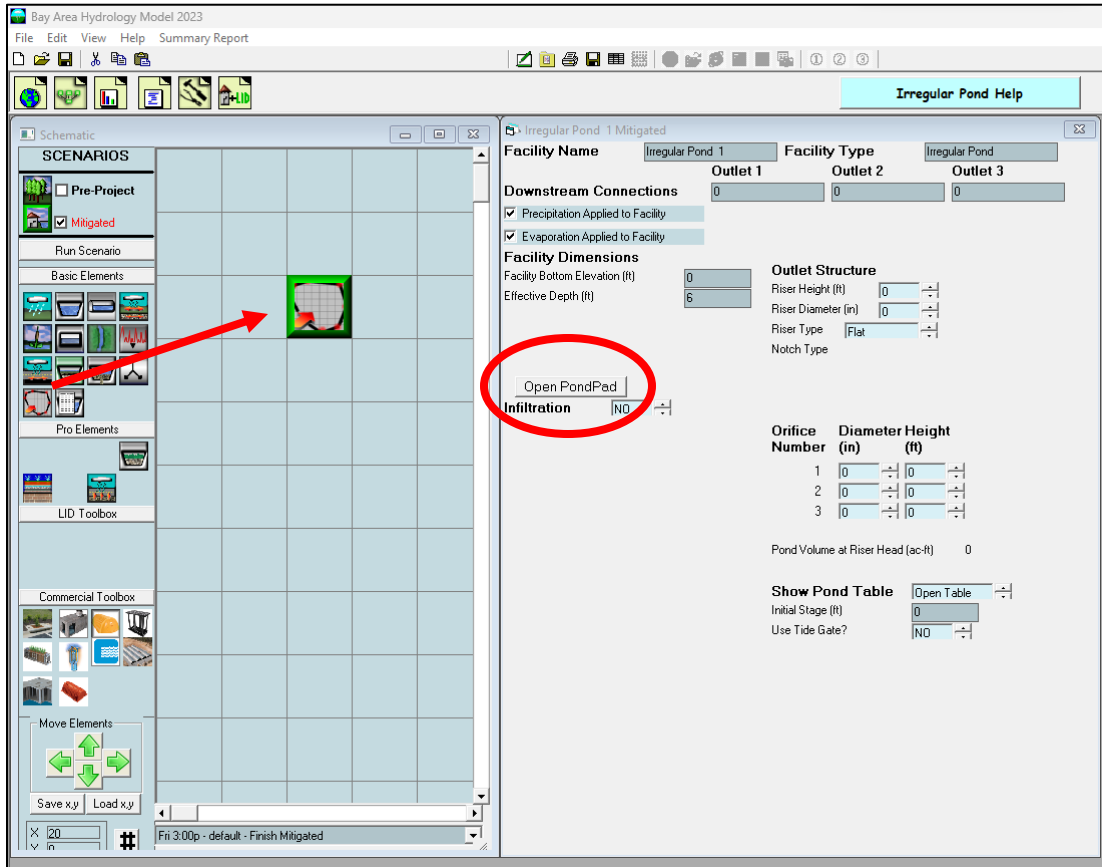


An irregular pond is any pond with a shape that differs from the rectangular top of a trapezoidal pond. An irregular pond has all of the same characteristics of a trapezoidal pond, but its shape must be defined by the user.

The Auto Pond option is not available for an irregular-shaped pond. Go to page 46 to find information on how to manually size an irregular pond similar to a trapezoidal pond.



To create the shape of an irregular pond the user clicks on the “Open PondPad” button. This allows the user to access the PondPad interface (see below).

PondPad Interface

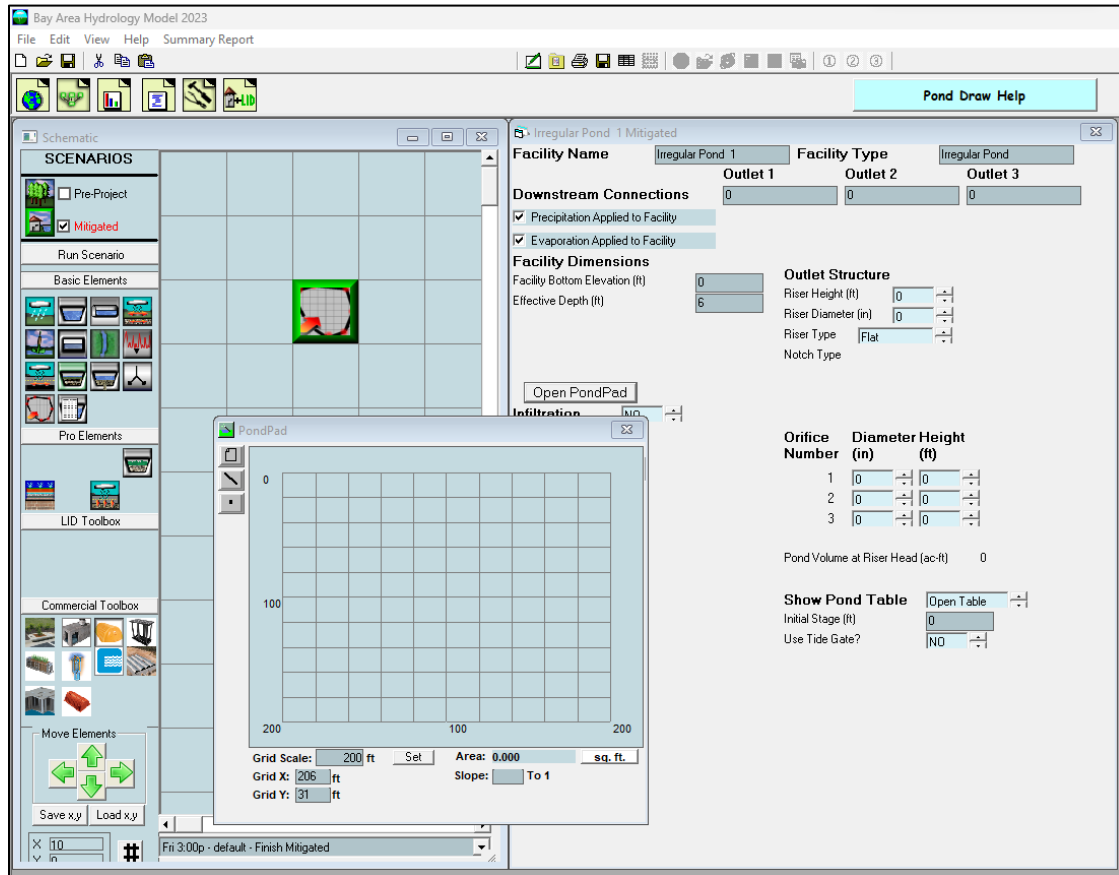

The PondPad interface is a grid on which the user can specify the outline of the top of the pond and the pond’s side slopes.

The user selects the line button (second from the top on the upper left corner of the PondPad screen). Once the line button is turned on the user moves the mouse over the grid to locate the pond’s corner points. The user does this in a clockwise direction to outline the pond’s top perimeter. The user can select individual points by clicking on the point button immediately below the line button. Once selected, any individual point can be moved or repositioned.

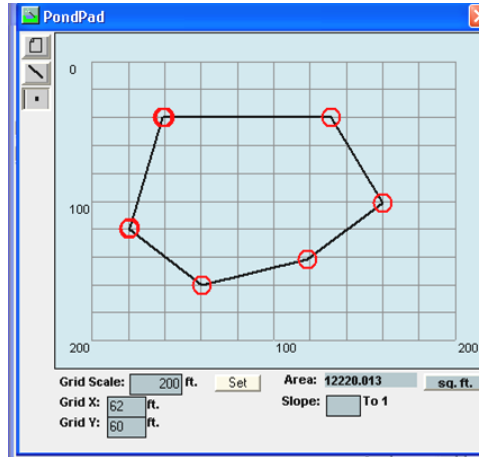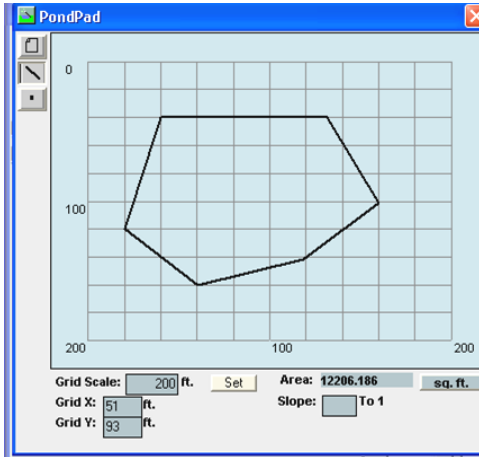

The default side slope value is 3 (3:1). The side slopes can be individually changed by right clicking on the specific side (which changes the line color from black to red) and then entering the individual side slope value in the slope text box.

The grid scale can be changed by entering a new value in the grid scale box. The default value is 200 feet.

PondPad Controls and Numbers


- Clear: The Clear button clears all of the lines on the grid.
- Line: The Line button allows the user to draw new lines with the mouse.
- Point: The Point button allows the user to move individual points to alter the pond shape and size.

- Sq Ft: Converts the computed pond area from square feet to acres and back.
- Grid Scale: Changes the length of a grid line. Default grid scale is 200 feet.
- Grid X: Horizontal location of the mouse pointer on the grid (0 is the upper left corner).
- Grid Y: Vertical location of the mouse pointer on the grid (0 is the upper left corner)

- Area: Top area of the pond (either in square feet or acres).
- Slope: Side slope of the selected line (side of the pond).

Learn more about the BAHM PondPad here:
www.clearcreeksolutions.info/bahm-course-home

GRAVEL TRENCH BED ELEMENT

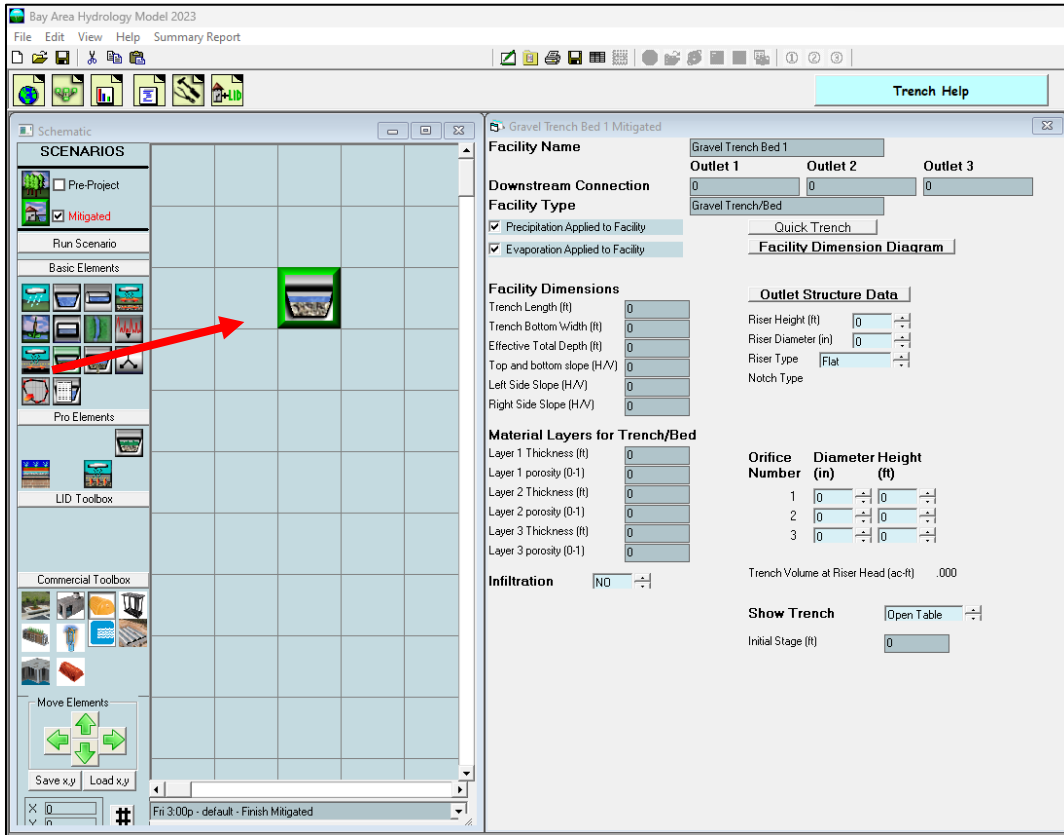

The gravel trench bed is used to spread and infiltrate runoff, but also can have one or more surface outlets represented by an outlet structure with a riser and multiple orifices.


The user specifies the trench length, bottom width, total depth, bottom slope, and left and right-side slopes.

The material layers represent the gravel/rock layers and their design characteristics (thickness and porosity).

Quick Trench will instantly create a gravel trench bed with default values without checking it for compliance with flow duration criteria.

The gravel trench bed input information:

- Trench Length (ft): Trench bed length.
- Trench Bottom Width (ft): Trench bed bottom width.

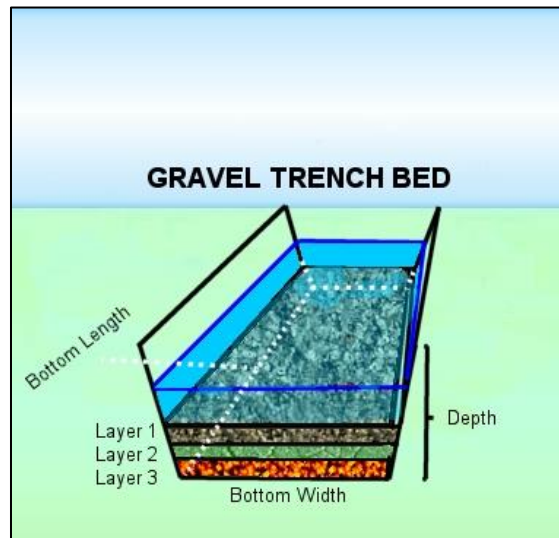

Effective Total Depth (ft): Height from bottom of trench bed to top of riser plus freeboard (at least 0.5 feet extra).

Bottom and Top Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical trench bed sides. Bottom and top side slopes are defined based on plan view.

Left Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical trench bed sides.

Right Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical trench bed sides.

Infiltration Rate (in/hr): Trench bed gravel or other media infiltration rate.

Layer 1 Thickness (ft): Trench top media layer depth.

Layer 1 Porosity: Trench top media porosity.

Layer 2 Thickness (ft): Trench middle media layer depth (Layer 2 is optional).

Layer 2 Porosity: Trench middle media porosity.

Layer 3 Thickness (ft): Trench bottom media layer depth (Layer 3 is optional).

Layer 3 Porosity: Trench bottom media porosity.

Riser Height (ft): Height of trench overflow pipe above trench bottom.

Riser Diameter (in): Trench overflow pipe diameter.

Riser Type (options): Flat or Notched

Notch Type: Rectangular, V-Notch, or Sutro.

For a rectangular notch:

Notch Height (feet): distance from the top of the weir to the bottom of the notch.

Notch Width (feet): width of notch; cannot be larger than the riser circumference.

For more information on riser notch options and orifices see discussion in OUTLET STRUCTURE CONFIGURATIONS section.

Native Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

Infiltration Reduction Factor: 1/Native soil infiltration rate safety factor (see page 123).

Use Wetted Surface Area (sidewalls): Yes, if infiltration through the trench side slopes is allowed.


If infiltration is used, then the user should consult the Infiltration discussion on page 123.

The infiltration trench does not explicitly include an underdrain. However, to include an underdrain, set the underdrain height and orifice diameter using the orifice input (the orifice height is defined as from the bottom of the lowest layer in the trench).

Gravel trench bed receives precipitation on and evaporation from the trench surface. The Precipitation Applied to Facility and Evaporation Applied to Facility boxes should be checked.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

SAND FILTER ELEMENT

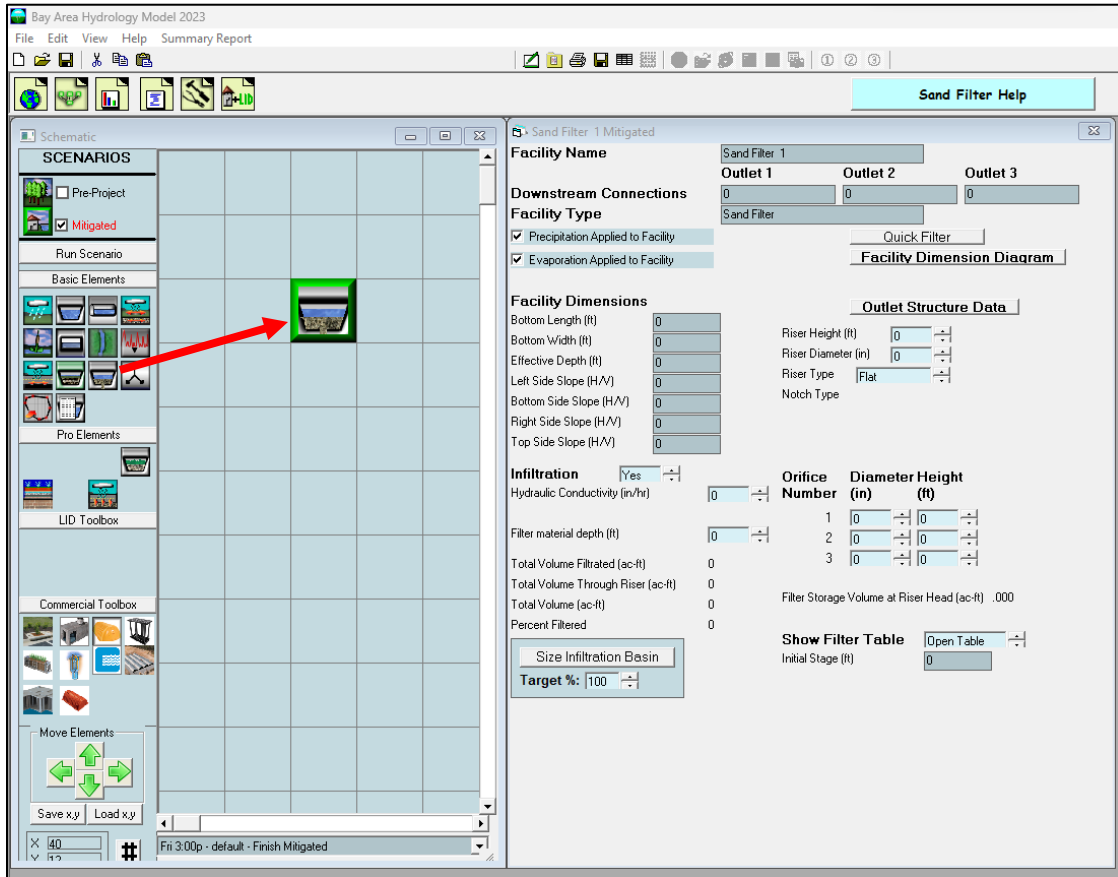


The sand filter is a water quality facility. It does not infiltrate runoff, but is used to filter runoff through a medium and send it downstream. It can also have one or more surface outlets represented by an outlet structure with a riser and multiple orifices.

The user must specify the facility dimensions (bottom length and width, effective depth, and side slopes). The hydraulic conductivity of the sand filter and the filter material depth are also needed to size the sand filter (default values are 1.0 inch per hour and 1.5 feet, respectively).

NOTE: The sand filter element is not acceptable as a stand-alone treatment measure in the Bay Area but may be used as a pre-treatment measure.

The filter discharge is calculated using the equation $Q = K \cdot I \cdot A$, where Q is the discharge in cubic feet per second (cfs). K equals the hydraulic conductivity (inches per hour). For

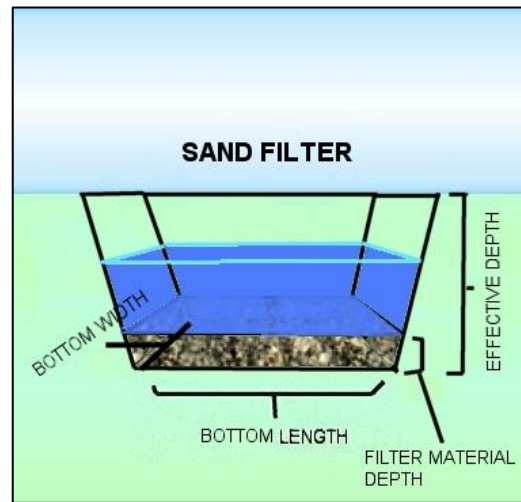

sand filters $K = 1.0$ in/hr. Sand is the default medium. If another filtration material is used then the design engineer should enter the appropriate K value supported by documentation and approval by the reviewing authority.

Design of a sand filter requires input of facility dimensions and outlet structure characteristics, running the sand filter scenario, and then checking the volume calculations to see if the Percent Filtered equals or exceeds the treatment standard percentage. If the value is less than the treatment standard percentage then the user should increase the size of the sand filter dimensions and/or change the outlet structure. The sand filter input information:

Bottom Length (ft): Sand filter bottom length.

Bottom Width (ft): Sand filter bottom width.

Effective Depth (ft): Height from bottom of sand filter to top of riser plus freeboard (at least 0.5 feet extra).

Left Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical sand filter sides.

Bottom Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical sand filter sides.

Right Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical sand filter sides.

Top Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical sand filter sides.

Riser Height (ft): Height of sand filter overflow pipe above sand filter surface.

Riser Diameter (in): Sand filter overflow pipe diameter.

Riser Type (options): Flat or Notched

Notch Type: Rectangular, V-Notch, or Sutro.

For a rectangular notch:

Notch Height (feet): distance from the top of the weir to the bottom of the notch.

Notch Width (feet): width of notch; cannot be larger than the riser circumference.

For more information on riser notch options and orifices see discussion in **OUTLET STRUCTURE CONFIGURATIONS** section.

Infiltration: Yes (infiltration through the filter material)


Hydraulic Conductivity (in/hr): Filtration rate through the sand filter.

Filter material depth (ft): Depth of sand filter material (for runoff filtration).

A sand filter receives precipitation on and evaporation from the sand filter surface. The Precipitation Applied to Facility and Evaporation Applied to Facility boxes should be checked.

Learn more about the Sand Filter element here:
www.clearcreeksolutions.info/bahm-course-home

CHANNEL ELEMENT

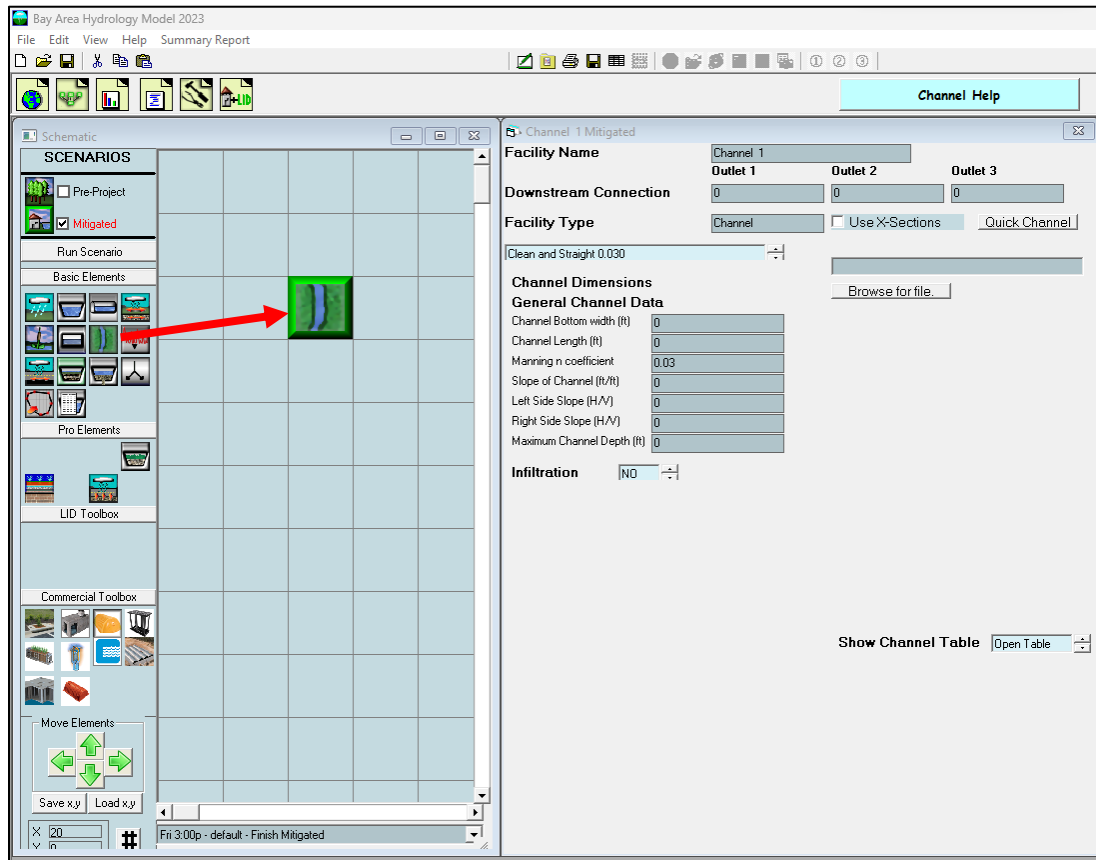


The Channel element allows the user to route runoff from a basin or facility through an open channel to a downstream destination.

The channel cross section is represented by a trapezoid and is used with Manning's equation to calculate discharge from the channel. If a trapezoid does not accurately represent the cross section, then the user should represent the channel with an independently calculated SSD Table element or use the Use X-Sections option. The user can learn more about X-Sections in the BAHM 2023 Helpfile.

The user inputs channel bottom width, channel length, channel bottom slope, channel left and right side slopes, maximum channel depth, and the channel's roughness coefficient (Manning's n value). The user can select channel type and associated Manning's n from a table list directly above the Channel Dimension information or directly input the channel's Manning's n value.

The channel is used to represent a natural or artificial open channel through which water is routed. It can be used to connect a basin to a pond or a pond to a pond or multiple channels can be linked together.

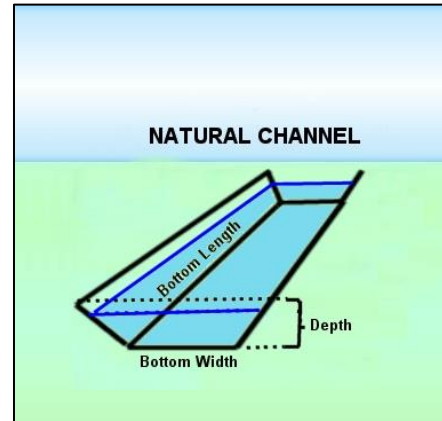

Channel input information:

Channel Bottom Width (ft): Open channel bottom width.

Channel Length (ft): Open channel length.

Manning's n coefficient: Open channel roughness coefficient (user menu selected or input).

Slope of Channel (ft/ft): Open channel bottom slope.

Left Side Slope of Channel (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical channel sides.

Right Side Slope of Channel (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical channel sides.

Maximum Channel Depth (ft): Height from bottom of channel to top of channel bank.

Infiltration: Yes (if the channel allows infiltration into the underlying native soil); No for concrete channel.

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

Infiltration Reduction Factor: 1/Native soil infiltration rate safety factor (see page 123).


Use Wetted Surface Area (sidewalls): Yes, if infiltration through the channel side slopes is allowed.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

Learn more about the Channel element here:
www.clearcreeksolutions.info/bahm-course-home


FLOW SPLITTER ELEMENT

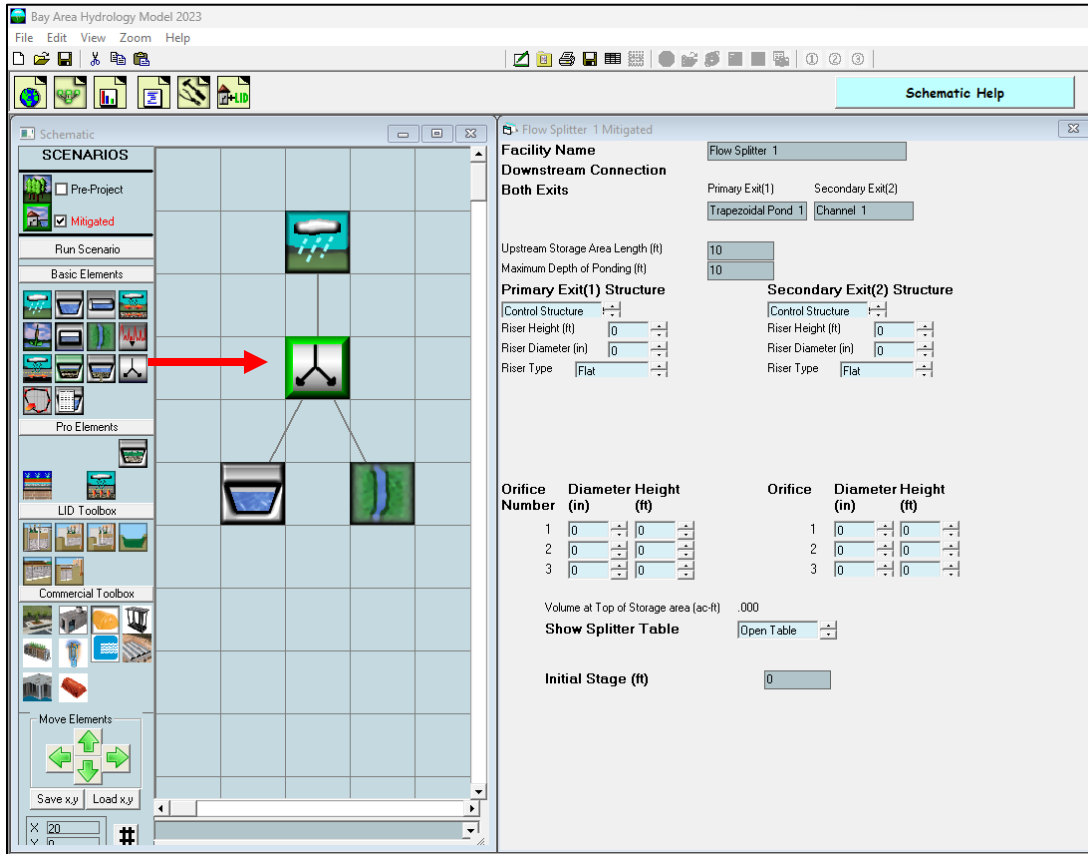

The flow splitter divides the runoff and sends it to two different destinations. The splitter has a primary exit (exit 1) and a secondary exit (exit 2). The user defines how the flow is split between these two exits.

There are two options for representing the flow splitter. The first option is that the user can define a flow control structure with a riser and one to three orifices for each exit. The flow control structure works the same way as the pond outlet structure, with the user setting the riser height and diameter, the riser weir type (flat, rectangular notch, V-notch, or Sutro), and the orifice diameter and height.


For more information on riser notch options and orifices see discussion in OUTLET STRUCTURE CONFIGURATIONS section.

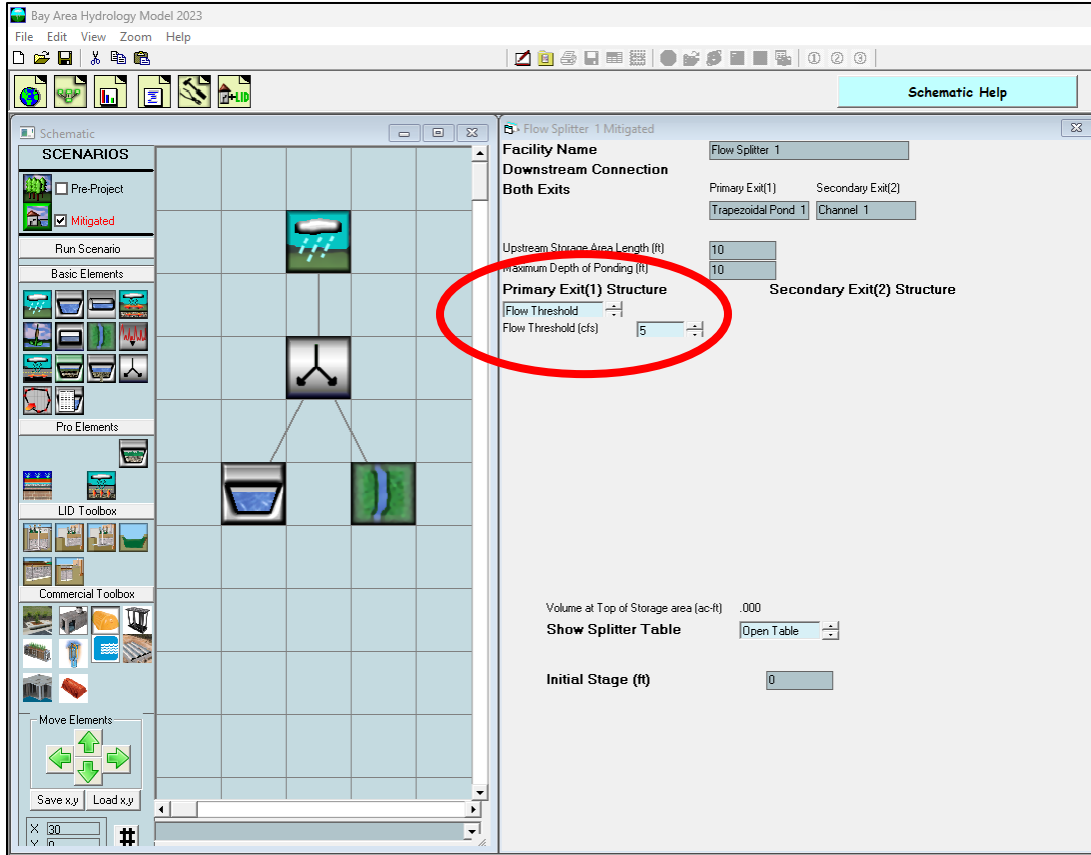

The second option is that the flow split can be based on a flow threshold. The user sets the flow threshold value (cfs) for exit 1 at which flows in excess of the threshold go to exit 2. For example, if the flow threshold is set to 5 cfs, then all flows less than or equal to 5 cfs go to exit 1. Exit 2 gets only the excess flow above the 5 cfs threshold (total flow minus exit 1 flow).

Learn more about the Flow Splitter element here:
www.clearcreeksolutions.info/bahm-course-home

TIME SERIES ELEMENT

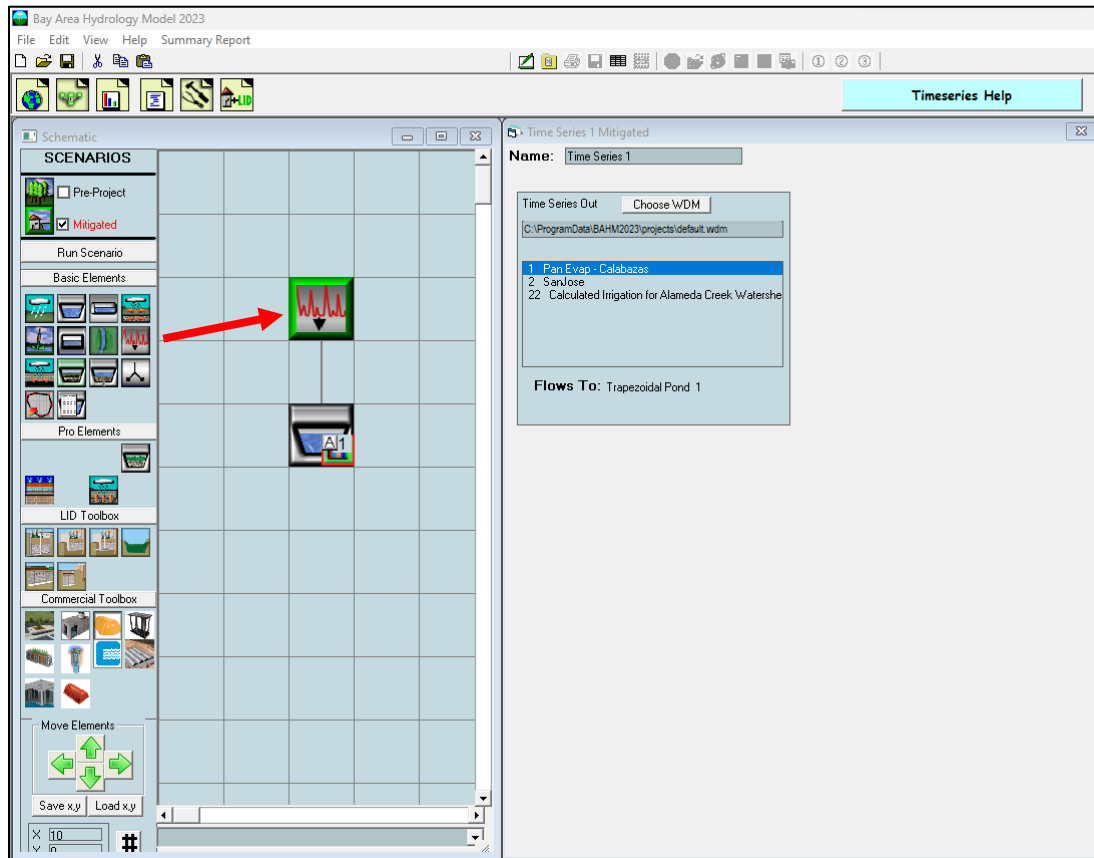


BAHM2023 uses time series of precipitation, evaporation, and runoff stored in its database (HSPF WDM file). The user has the option to create or use a time series file external from BAHM2023 in BAHM2023. This may be a time series of flow values created by another HSPF model. An example is offsite runoff entering a project site. If this offsite runoff is in an existing WDM file and is the same period as BAHM2023 data and the same simulation time step (hourly) then it can be linked to BAHM2023 model using the Time Series element.

To link the external time series to BAHM2023, the user clicks on the Choose WDM button and identifies the external WDM file. The external WDM's individual time series files are shown in the Time Series Out box. The selected input dataset is the time series that will be used by BAHM2023.

The user also has the option of modifying and/or copying time series files using the options shown in the Functions box. These options are: add, subtract, apply factor (multiply), copy, raise to a power, select a threshold greater than, and select a threshold less than. Once a specific option is selected then by clicking on Run Analysis the time series is appropriately modified.

SSD TABLE ELEMENT

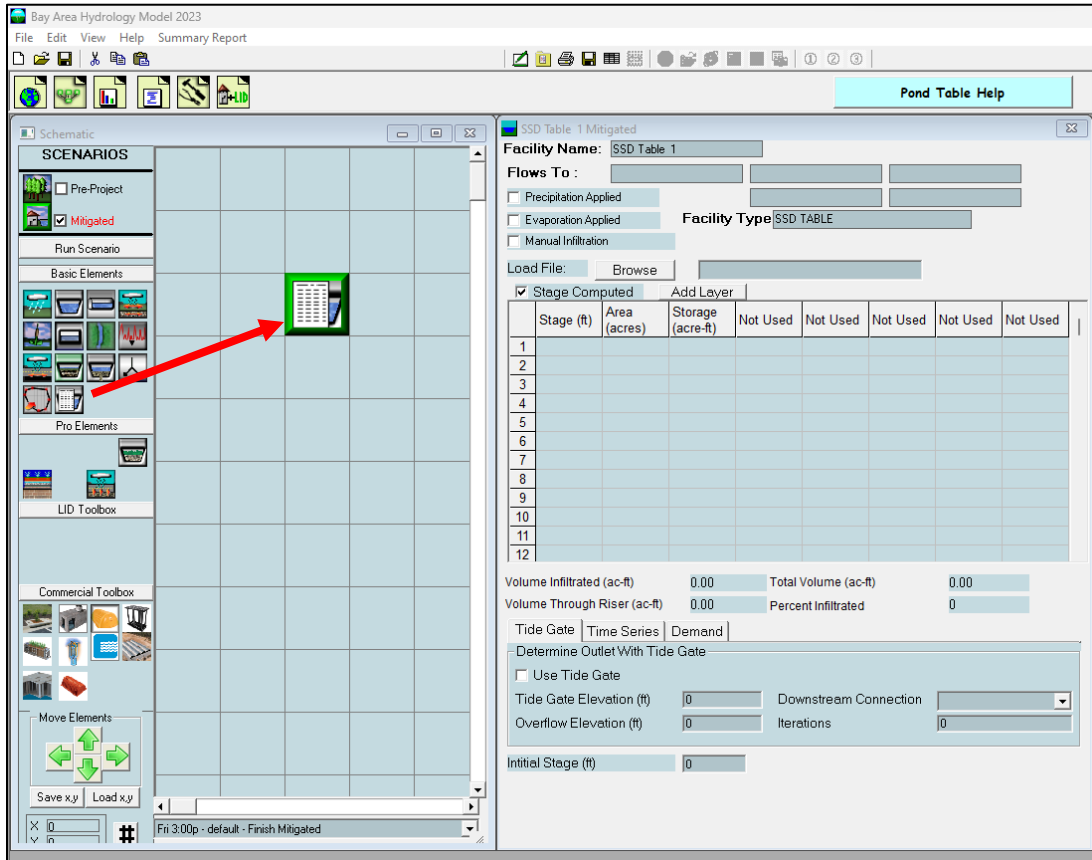

The SSD Table is a stage-storage-discharge table externally produced by the user and is identical in format to the stage-storage-discharge tables generated internally by BAHM2023 for ponds, vaults, tanks, and channels.

The easiest way to create an SSD Table outside of BAHM2023 is to use a spreadsheet with a separate column for stage, surface area, storage, and discharge (in that order). Save the spreadsheet file as a space or comma-delimited file. A text file can also be created, if more convenient.

The SSD Table must use the following units:

Stage: feet

Surface Area: acres

Storage: acre-feet

Discharge: cubic feet per second (cfs)

A fifth column can be used to create a second discharge (cfs). This second discharge can be infiltration or a second surface discharge.


Certain rules apply to the SSD Table whether it is created inside or outside of BAHM2023. These rules are:

1. Stage (feet) must start at zero and increase with each row. The incremental increase does not have to be consistent.
2. Storage (acre-feet) must start at zero and increase with each row. Storage values should be physically based on the corresponding depth and surface area, but BAHM2023 does not check externally generated storage values.
3. Discharge (cfs) must start at zero. Discharge does not have to increase with each row. It can stay constant or even decrease. Discharge cannot be negative. Discharge should be based on the outlet structure's physical dimensions and characteristics, but BAHM2023 does not check externally generated discharge values.
4. Surface area (acres) is only used if precipitation to and evaporation from the facility are applied.


To input an externally generated SSD Table, first create and save the table outside of BAHM2023. Use the Browse button to locate and load the file into BAHM2023.

Save the spreadsheet file as a comma-delimited file. A text file can also be created, if more convenient.


More information on stage-storage-discharge tables, in general, can be found starting page 127.

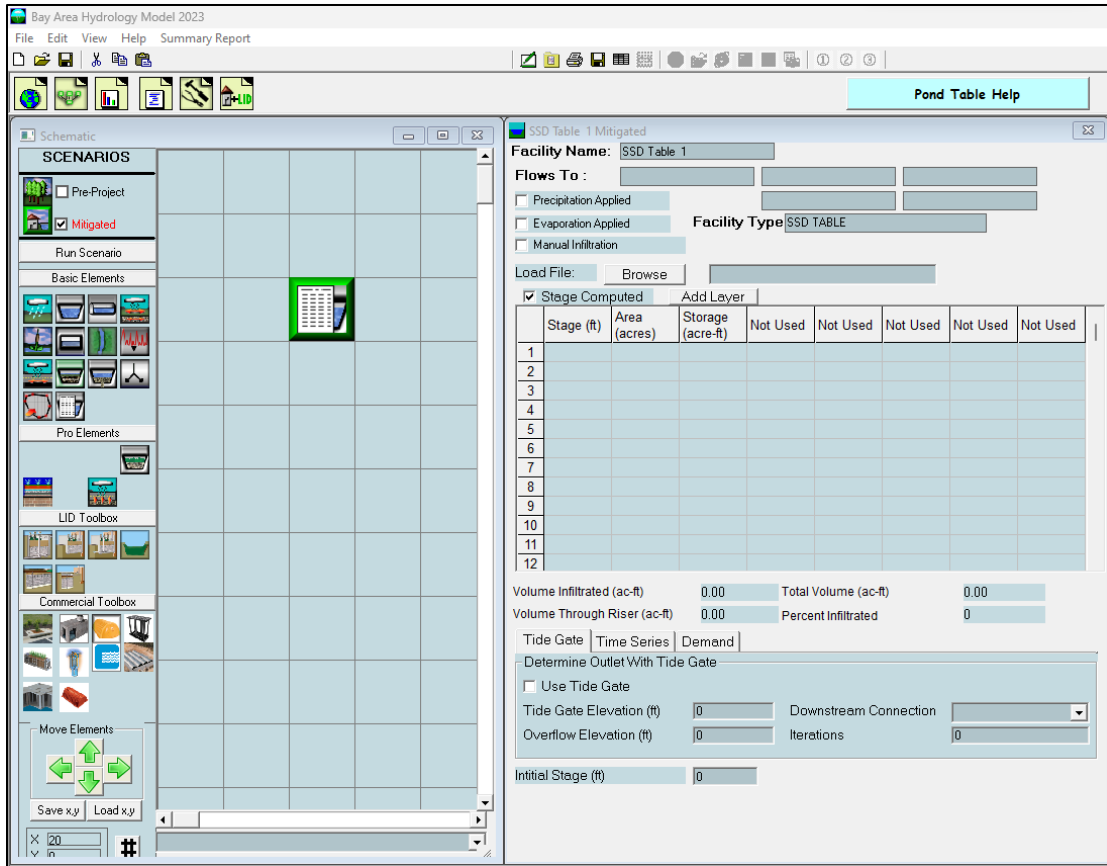

Custom values can also be input into the SSD Table. To input columns of values beyond (to the right of) the Storage column click on the “Not Used” title and select the appropriate option. Use “Manual” when the discharge has been included in the external spreadsheet.

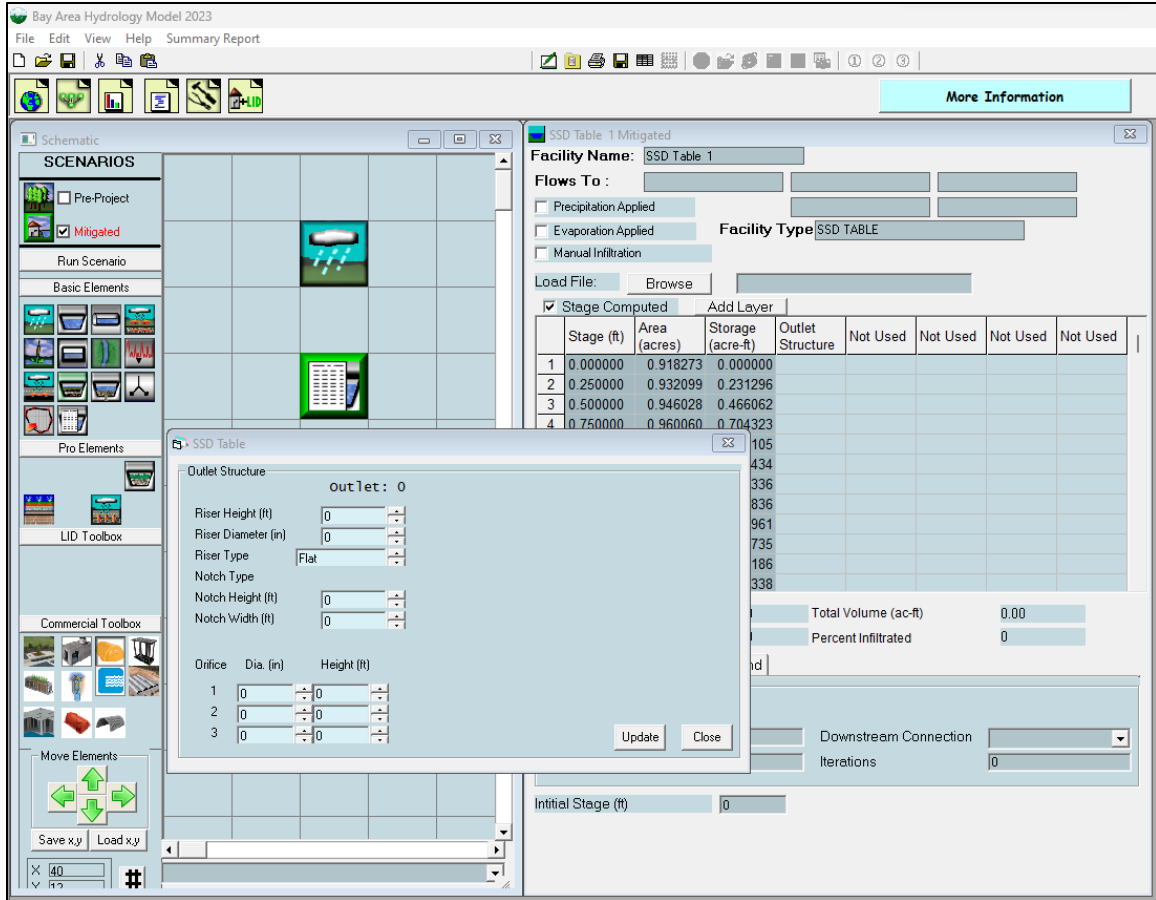


Use “Outlet Structure” to input riser and orifice dimensions.

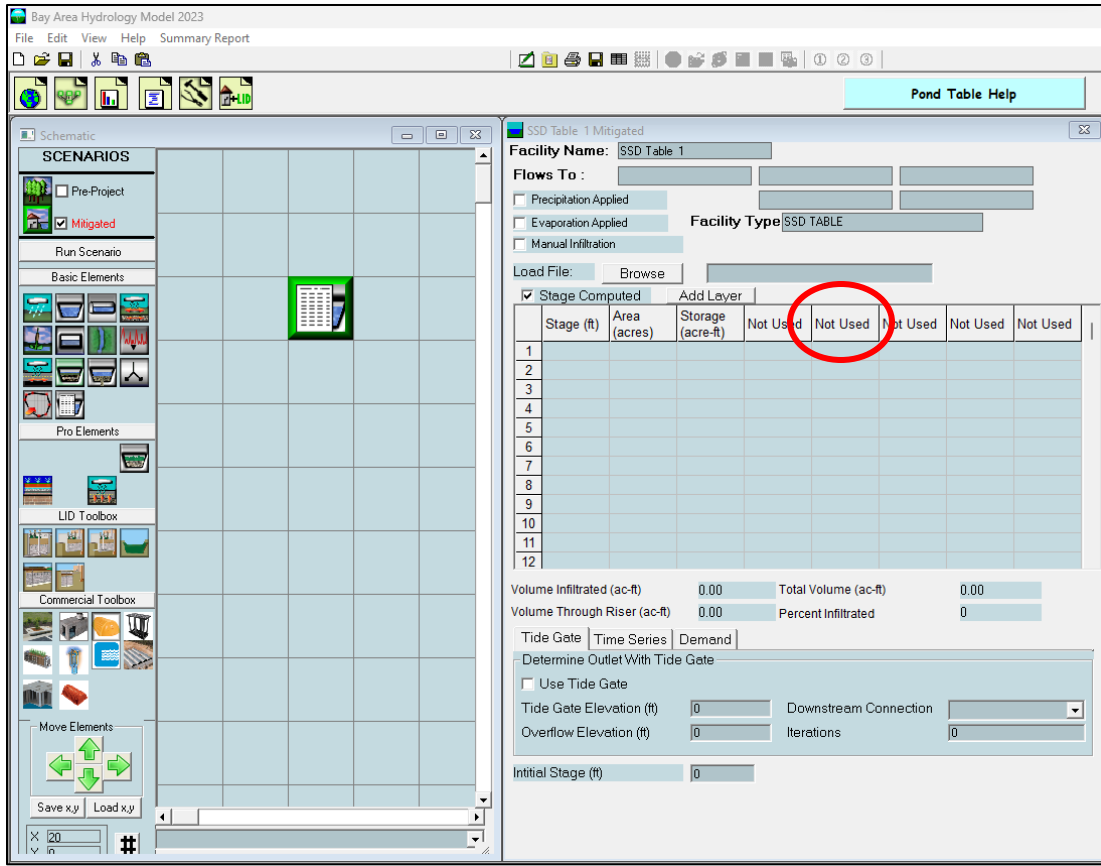

The fifth column can be used for a second surface outlet (manual or outlet structure), infiltration, or aquifer recharge. Aquifer recharge differs from infiltration in how the model separately accounts for it.

Learn more about the SSD Table element here:
www.clearcreeksolutions.info/bahm-course-home

HIGH GROUNDWATER/WETLAND ELEMENT

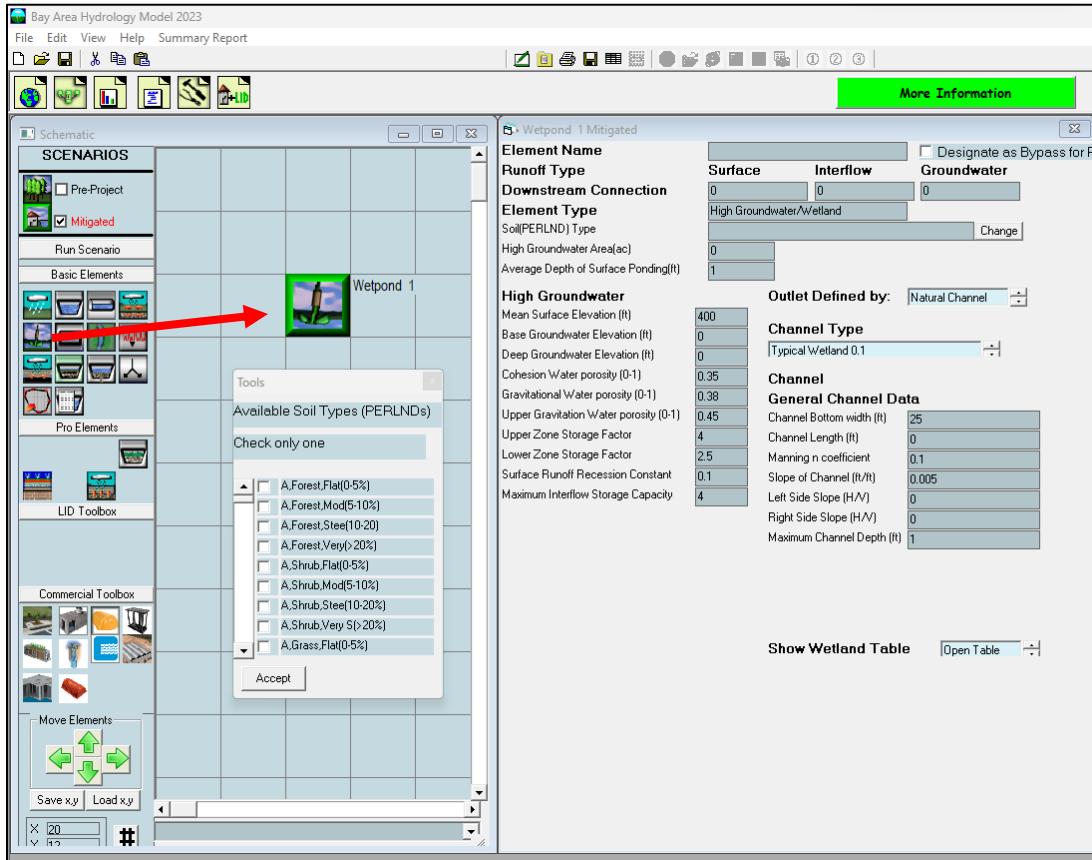

The High Groundwater/Wetland element is a complex element that should only be used in special applications by advanced BAHM2023 users. The purpose of the high groundwater/ wetland element is to model hydrologic conditions where high groundwater rises to the surface (or near the surface) and reduces the ability of water to infiltrate into the soil.

The element can be used to represent wetland conditions with surface ponding where the discharge from the wetland is via a surface release. The user is given the choice of using either a natural channel, berm/weir, or control structure to determine the release characteristics.

The element provides default values for some of the parameters, especially as they relate to high groundwater. The user should be fully familiar with these parameters and the appropriate values for their site prior to attempting to use this element. The high groundwater parameter definitions are shown below.

Cohesion water porosity: soil pore space in micropores.

Gravitational water porosity: soil pore space in macropores in the lower and groundwater layers of the soil column.

Upper gravitation water porosity: soil pore space in macropores in the upper layer of the soil column.

Upper zone storage factor: portion of the water stored in macropores in the upper soil layer which will not surface discharge, but will percolate, evaporate or transpire.

Lower zone storage factor: portion of the water stored in micropores in the lower soil layer which will not gravity drain, but will evaporate or transpire.

NOTE: Due to permit restrictions on infiltration for stormwater treatment measures in areas of high groundwater, consult with the local municipal permitting agency regarding any project conditions that might involve using this element.

Learn more about the High Groundwater element here:
www.clearcreeksolutions.info/bahm-course-home

LID ELEMENTS

The following pages contain information about these LID elements and options:

- Self-Retaining Area
- Bioretention
- In-Ground Planter
- Flow-Through Planter
- Permeable Pavement
- Dispersion
- Lateral Flow Soil Basin (Pervious)
- Lateral Flow Impervious Area (Impervious)
- Dry Well
- Infiltration Trench
- Infiltration Basin
- Green Roof
- Rainwater Harvesting

Learn more about LID Elements here:
www.clearcreeksolutions.info/bahm-course-home

SELF-RETAINING AREA

What is a Self-Retaining Area?

A self-retaining area is a pervious area that can receive and treat stormwater runoff from adjacent impervious areas. The self-retaining area is primarily used for water quality treatment, and it may have a small effect on water quantity as well; however, a self-retaining area should not be considered a hydromodification control measure by itself.

In order to use a self-retaining area, you will need to compute the ratio of contributing impervious area to self-retaining (pervious) area. The maximum allowed ratio to meet treatment requirements given Bay Area soil conditions is 2 to 1. This means that for every acre of contributing impervious area, you will need 0.5 acres of self-retaining area. The self-retaining area should be a flat area that is slightly depressed such that it can retain up to 3 inches of runoff. This value can change based on the ratio of impervious to pervious area. Table 1 below shows the required depth for each associated ratio.

Table 1. Self-Retaining Area Input

Impervious/Pervious Ratio of Area	Depth of impoundment feet (in)
2	0.25 (3)
1.5	0.1875 (2.25)
1	0.125 (1.5)
0.5	0.0625 (0.75)

How to Model a Self-Retaining Area

A self-retaining area is represented in BAHM as a very shallow pond. To properly model a self-retaining area, the user will need to follow these steps.

- 1) Determine the ratio of upstream contributing impervious area to the pervious self-retaining areas.
- 2) Based on this ratio, determine the depth in inches required.
- 3) Place an upstream contributing basin element.
- 4) Enter the land use area.
- 5) Place a trapezoidal pond element in the schematic.
- 6) The user will need to enter the following attributes into the pond element:
 - a. Surface area (length X width) = self-retaining area.
 - b. Depth of facility = 2 feet.
 - c. Side slopes = 0
 - d. Riser height = required depth of impoundment from Table 1.
 - e. Riser diameter = 2 times the weir flow length of the self-retaining area.
This is basically 2 times the length of the edge where water will overflow the self-retaining area.
 - f. Notch height = 2 minus the required depth of impoundment from Table 1.

- g. Notch width = the weir flow length of the self-retaining area. This represents the length of the edge where water will overflow the self-retaining area.
- h. Set infiltration = 0.1 inches/hour.

Modeling Example

1. Determine the ratio of contributing impervious area and to the self-retaining area. For this example, the self-retaining area is 66’ x 66’ = 0.1 acres. The upstream contributing impervious area is 0.2 acres. $0.2/0.1 = \text{Ratio of } 2$
2. Based on this ratio, the user will determine the depth of impoundment in feet required. For this example, it is 0.25 ft. Additionally, it is necessary to input 2 ft for the effective depth to allow the model to handle overflows.


Facility Dimensions	
Facility Bottom Elevation (ft)	0
Bottom Length (ft)	66
Bottom Width (ft)	66
Effective Depth (ft)	2

3. Then place an upstream contributing impervious basin element.

Area in Basin		Available Impervious	
Available Pervious	Acres	Acres	Acres
<input checked="" type="checkbox"/> A.Forest.Flat(0-5%)	0	<input checked="" type="checkbox"/> Roads.Flat(0-5%)	2
<input type="checkbox"/> A.Forest.Mod(5-10%)	0	<input type="checkbox"/> Roads.Mod(5-10%)	0
<input type="checkbox"/> A.Forest.Stee(10-20%)	0	<input type="checkbox"/> Roads.Stee(10-20%)	0
<input type="checkbox"/> A.Forest.Very(>20%)	0	<input type="checkbox"/> Roads.VeryStee(>20%)	0
<input type="checkbox"/> A.Shrub.Flat(0-5%)	0	<input type="checkbox"/> Flood Area	0
<input type="checkbox"/> A.Shrub.Mod(5-10%)	0	<input type="checkbox"/> Driveways.Flat(0-5%)	0
<input type="checkbox"/> A.Shrub.Stee(10-20%)	0	<input type="checkbox"/> Driveways.Mod(5-10%)	0
<input type="checkbox"/> A.Shrub.Very S(>20%)	0	<input type="checkbox"/> Driveways.St(10-20%)	0
<input type="checkbox"/> A.Grass.Flat(0-5%)	0	<input type="checkbox"/> Driveways.Very(>20%)	0
<input type="checkbox"/> A.Grass.Mod(5-10%)	0	<input type="checkbox"/> Sidewalks.Flat(0-5%)	0
<input type="checkbox"/> A.Grass.Stee(10-20%)	0	<input type="checkbox"/> Sidewalks.Mod(5-10%)	0
<input type="checkbox"/> A.Grass.Very S(>20%)	0	<input type="checkbox"/> Sidewalks.St(10-20%)	0
<input type="checkbox"/> A.Urban.Flat(0-5%)	0	<input type="checkbox"/> Sidewalks.Very(>20%)	0
<input type="checkbox"/> A.Urban.Mod(5-10%)	0	<input type="checkbox"/> Parking.Flat(0-5%)	0
<input type="checkbox"/> A.Urban.Stee(10-20%)	0	<input type="checkbox"/> Parking.Mod(5-10%)	0
<input type="checkbox"/> A.Urban.Very S(>20%)	0	<input type="checkbox"/> Parking.Stee(10-20)	0
<input type="checkbox"/> B.Forest.Flat(0-5%)	0	<input type="checkbox"/> Parking.Very(>20%)	0
<input type="checkbox"/> B.Forest.Mod(5-10%)	0	<input type="checkbox"/> Porous Pavement	0
<input type="checkbox"/> B.Forest.Stee(10-20)	0		
<input type="checkbox"/> B.Forest.Very(>20%)	0		
<input type="checkbox"/> B.Shrub.Flat(0-5%)	0		

Pervious Total: 0 Acres
 Impervious Total: 0.2 Acres
 Basin Total: 0.2 Acres

4. Enter the landuse area for the basin. 0.2 acres of upstream impervious area was added to the basin.
5. Now place a trapezoidal pond element in the mitigated scenario. Connect the basin to the trapezoidal pond and add an “Analyze” marker to the pond element.

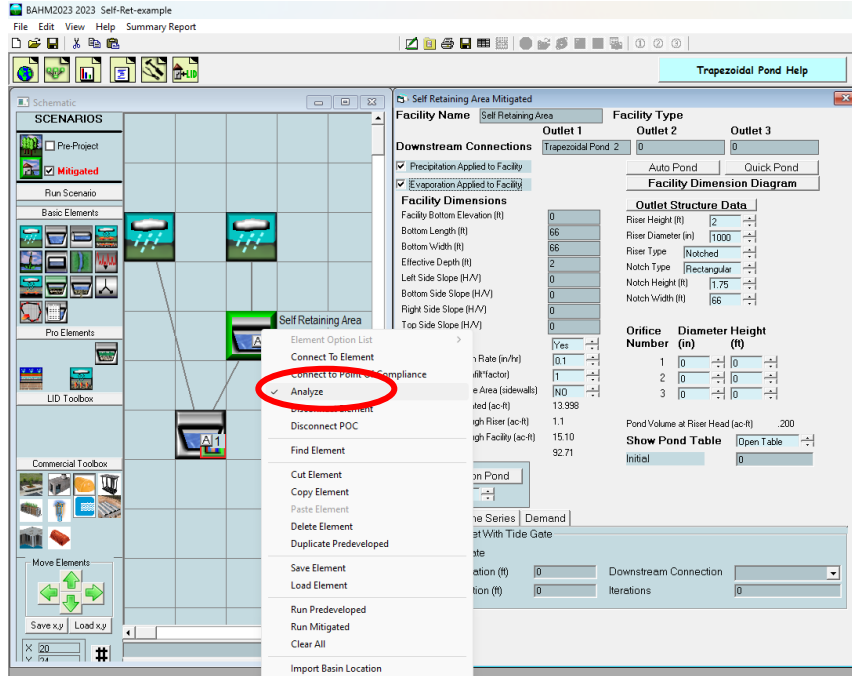


6. Enter the following parameters into the trapezoidal pond element, that is now our self-retaining area.
 - a. Surface area of length X width. For this example, it will be 66' by 66'.
 - b. The depth of the facility will be 2 feet. Enter this value into the “Facility Depth” column of the pond element as seen below.
 - c. Enter all the side slopes of the facility to be “0”, as seen below.

- d. Set the riser height to be 2 feet.
- e. Riser diameter = 2 times the weir flow length of the self-retaining area. This is basically 2 times the length of the edge where water will overflow the self-retaining area. For this example, it will be 1000 inches, or approximately 83 feet.
- f. Notch height = 2 minus the required depth of impoundment from Table 1. For this example, it will be 1.75 feet. $2 - 0.25 = 1.75$ ft.
- g. Notch width = the weir flow length of the self-retaining area. This represents the length of the edge where water will overflow the self-retaining area. For this example, it will be 66 feet.
- h. Set infiltration = 0.1 inches/hour.

Learn more about the Self-Retaining Area element here:
www.clearcreeksolutions.info/bahm-course-home

BIORETENTION ELEMENT

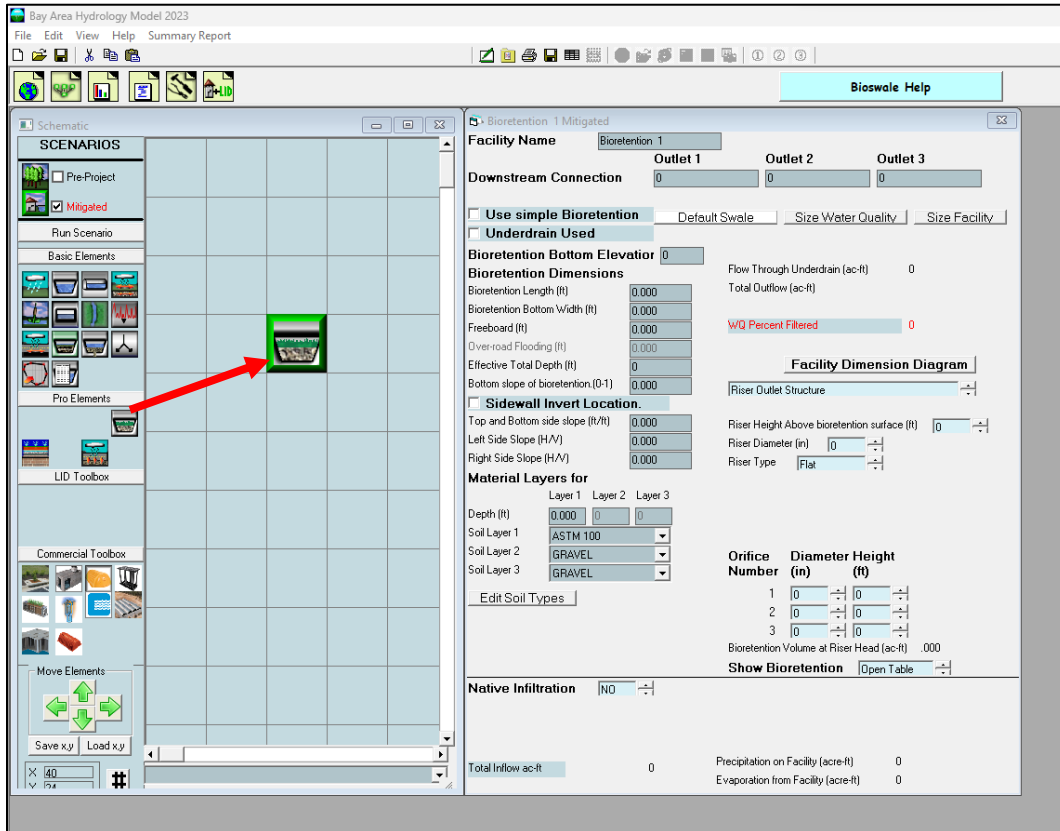

The bioretention element is a landscaped treatment system in which the native soils have been excavated and replaced with engineered soil. The bioretention element is represented as a depression filled with one to three layers of amended soil and gravel. The amended soil layer(s) provide runoff treatment by filtering the runoff. It can also have one or more surface outlets represented by an outlet structure with a riser and multiple orifices, or a vertical orifice and weir overflow structure.

The surface area of the Bioretention cannot be a part of the Drainage Management Area, and may have to be subtracted from the mitigated landuse area.

The material layers represent the amended soil(s) and gravel and their design characteristics (thickness and vertical water movement). These are the engineered soil layers added to the bioretention facility to filter the runoff prior to dispersal.

The bioretention element can be run with a complex routing option or with a simple option.

The complex option runs a special internal check that is performed every time step by the model during the course of the model run. This internal check evaluates the total available storage in the soil layers and computes the total discharge from the soil layers through either native infiltration or flow through the underdrain and the total inflow and compares this to the total available inflow into the soil layers. If the inflow exceeds the available volume plus the outflow, then the inflow is reduced to match.

The simple option (“Simple Bioretention”) turns off the special internal check, which results in a faster computation time. This option is good for most model run scenarios and is recommended for general use.

There is one scenario where the more complex routing option is recommended. If the discharge from the facility is likely to be restrictive and cause the facility to fill all the soil layers and not allow inflow from the surface, then it is recommended that the complex option be used.

The complex option is most likely to be required under these conditions:

- 1) The only discharge is to native infiltration and the native infiltration rate is lower than the filtration rate through the soil layers.
- 2) The only discharge is through the underdrain and the underdrain has a restrictive orifice that causes backwater.
- 3) Both the native infiltration and the underdrain are turned on, but the combined outflow is still restrictive enough to cause a backwater condition.

If these conditions are not present, then the simple option will produce the same results as the complex option.

The BAHM2023 bioretention element uses the HSPF hydraulic algorithms to route runoff, but the HSPF routing is modified to represent the two different flow paths that runoff can take. The routing is dependent on the inflow to the bioretention element and the engineered and native soils’ capacity to absorb additional runoff. HSPF Special Actions is used to check the soil capacity to determine the appropriate routing option.

Infiltration from the engineered soil to the native soil is also possible, depending on the properties of the native soil. Bioretention facilities can include an underdrain pipe at a specified depth. There is no underdrain for A or B soils.


The material layers represent the engineered “soils” (i.e., soil layer(s) and gravel) and their design characteristics (thickness and vertical water movement). Each engineered soil type has appropriate drainage characteristics assigned based on literature values. When a soil type is selected by the user, then BAHM2023 automatically assigns the appropriate values for:

1. Wilting: wilting point (0-1)
2. Porosity: saturated moisture content (0-1)
3. K Sat: maximum saturated hydraulic conductivity (cm/hr)
4. VG n: Van Genuchten number (from literature)
5. A: alpha (constant)
6. L: lambda (constant)
7. BPH: bubbling pressure head (cm)

The user can see the values for any of the soil types by selecting the soil type from the pulldown menu:

If none of the available soil types represents the engineered soil planned for use on the site, then the user can select a new soil type and input the appropriate values into the above input table.

NOTE: All bioretention-type facilities used in the Bay Area must use the biotreatment soil mix specified in the Municipal Regional Stormwater Permit (MRP) for the top layer (see “Revised Model Biotreatment Soil Media Specifications”, BASMAA, 2016 for more details). This biotreatment soil mix is represented by “BAHM 5”, which contains the appropriate soil values to meet the specification.

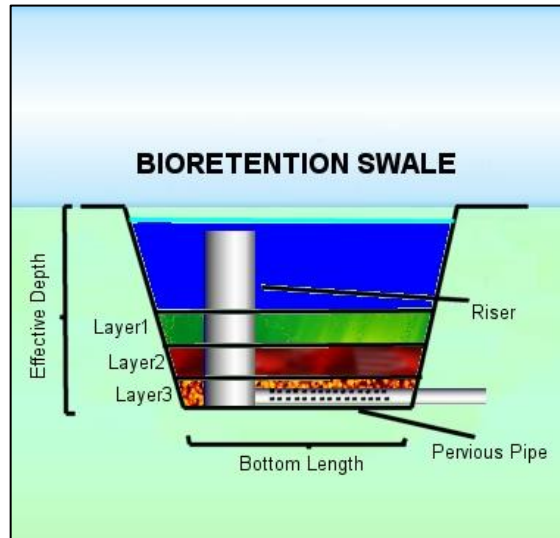

The first engineered soil layer should be the BAHM 5 soil mix specified by the Municipal Regional Stormwater Permit.

The second engineered soil layer is an intermediate material that is intended to prevent loss of fine material out of the engineered top layer soil mix into the gravel underlayer (layer 3). This layer is optional.

The third (bottom) engineered soil layer should be gravel.

A full list of the soil mixtures included in BAHM2023 is shown in Table 1.

Table 1. BAHM2023 Soil Mixtures

Soil Type	Wilting Point	Porosity	VG n	Ksat (cm/hr)	A	L	BPH
BAHM 5*	0.0700	0.450	1.700	12.70	6.90	1.30	7.90
GRAVEL	0.0050	0.420	10.000	1260.00	0.50	1.19	0.20
Sand	0.0200	0.420	3.000	23.56	6.00	0.69	7.26
Gravel Loamy Sand	0.1000	0.450	3.500	570.97	4.00	2.50	5.00
Coarse sand	0.0520	0.395	3.162	23.56	6.26	2.16	7.26
Humous loamy mcs	0.0600	0.470	2.348	15.00	6.50	1.35	7.50
Light loamy mcs	0.0600	0.394	2.145	10.00	6.50	1.14	7.50
Medium coarse sand (mcs)	0.0820	0.365	2.959	18.00	6.50	1.96	7.50
Loamy mcs	0.0600	0.301	1.941	9.00	7.00	0.94	8.00
Medium fine sand	0.0970	0.350	2.755	11.00	7.00	1.76	8.00
Fine sand	0.0520	0.364	2.552	10.00	7.30	1.55	8.30
Loamy fine sand	0.0600	0.439	1.738	2.18	7.69	0.74	8.69
Loam	0.0560	0.503	1.479	1.32	10.15	0.48	11.15
Sandy loam	0.0350	0.437	1.445	5.98	7.69	0.55	8.69
Fine sandy loam	0.0560	0.504	1.660	1.10	15.00	0.66	16.00
Clay loam	0.0875	0.445	1.413	0.20	24.89	0.41	25.89
Sandy clay loam	0.0665	0.432	1.318	0.30	27.08	0.32	28.08
Silty clay loam	0.0770	0.475	1.514	0.20	31.56	0.51	32.56
Silty clay	0.0980	0.507	1.318	0.10	33.19	0.32	34.19
Clay	0.0980	0.507	1.318	0.06	33.19	0.32	34.19
Peat	0.0995	0.863	3.050	0.15	39.00	2.05	40.00
Amended 1.5 in/hr	0.0850	0.450	1.400	5.00	7.30	0.85	8.30
Amended 2.5 in/hr	0.0800	0.470	1.500	6.50	7.20	0.90	8.20
Amended 3.0 in/hr	0.0750	0.480	1.600	7.62	7.10	1.00	8.10
Amended 5 in/hr	0.0700	0.490	2.200	13.00	6.90	1.30	7.90
SMMWW**	0.0650	0.850	3.000	15.24	6.50	1.40	7.50
Amended 15 in/hr	0.0600	0.480	3.200	39.00	6.30	2.10	7.30
ASTM 1	0.0900	0.410	1.500	2.54	7.50	0.75	8.50
ASTM 2	0.0825	0.420	1.550	5.08	7.30	0.88	8.30
ASTM 3	0.0750	0.430	1.600	7.62	7.10	1.00	8.10
ASTM 4	0.0725	0.440	1.650	10.16	7.00	1.15	8.00
ASTM 5	0.0700	0.450	1.700	12.70	6.90	1.30	7.90
ASTM 6	0.0675	0.460	1.850	15.24	6.50	1.40	7.50
ASTM 7	0.0667	0.470	2.000	17.78	6.45	1.50	7.45
ASTM 8	0.0659	0.480	2.150	20.32	6.43	1.58	7.43
ASTM 9	0.0651	0.490	2.300	22.86	6.41	1.66	7.41
ASTM 10	0.0643	0.500	2.450	25.40	6.39	1.74	7.39
ASTM 11	0.0635	0.510	2.600	27.94	6.37	1.82	7.37
ASTM 12	0.0627	0.520	2.750	30.48	6.35	1.90	7.35
ASTM 13	0.0619	0.530	2.900	33.02	6.33	1.98	7.33
ASTM 14	0.0611	0.540	3.050	35.56	6.31	2.06	7.31
ASTM 15	0.0603	0.550	3.200	39.00	6.30	2.14	7.30
ASTM 24.32	0.0590	0.550	3.200	39.00	6.25	2.25	7.20
ASTM 35.46	0.0550	0.550	3.250	90.10	6.20	2.30	7.00
ASTM 50	0.0500	0.550	3.300	127.00	6.15	2.35	6.80

Soil Type	Wilting Point	Porosity	VG n	Ksat (cm/hr)	A	L	BPH
ASTM 60	0.0490	0.550	3.350	152.40	6.10	2.40	6.40
ASTM 100	0.0450	0.550	3.400	254.00	6.05	2.45	6.00

*BAHM 5 is the San Francisco Bay Municipal Regional Permit required top layer standard soil mix for bioretention facilities.

**SMMWW is the Washington State Department of Ecology required top layer standard soil mix for bioretention facilities.

Wilting: wilting point (0-1)

Porosity: saturated moisture content (0-1)

K Sat: maximum saturated hydraulic conductivity (cm/hr)

VG n: Van Genuchten number (from literature)

A: alpha (constant)

L: lambda (constant)

BPH: bubbling pressure head (cm)

Table 1 values are from Schaap and Leij, 1998 soil parameter estimations using Rosetta.

The water movement through the soil column calculations are based on the methodology described in Appendix E: Bioretention Modeling Methodology.

The native soil infiltration is input by the user and is assumed to be constant throughout the year.

Inflow to the bioretention facility can exceed the engineered soil infiltration rate. When this occurs, the extra water ponds on the surface of the bioretention area. The extra water can then infiltrate into the soil during the next time step or can flow out of the bioretention facility through its surface outlet if the ponding exceeds the surface storage.

Runoff in both the surface storage and engineered soil storage is available for evapotranspiration. Surface storage evapotranspiration is set to the potential evapotranspiration; the engineered soil evapotranspiration pan evaporation coefficient is set to 0.50 to reflect reduced evapotranspiration from the engineered soil.

The user is required to enter the following information about the bioretention facility:

The bioretention dimensions are specified in terms of bottom length, bottom width, freeboard, over-road flooding, effective total depth, bottom slope, and side slopes.

Bottom Length (ft): length dimension of surface bottom.

Bottom Width (ft): width dimension of surface bottom.

Freeboard (ft): height above riser to top of facility.

Over-road Flooding (ft): maximum depth of flow over weir/street (only required for vertical orifice plus overflow outlet).

Effective Total Depth (ft): the total depth of the engineered soil layer(s) plus riser height plus freeboard; effective total depth is computed by BAHM2023.

Bottom Slope (ft/ft): the slope of the bioretention facility length; must be greater than zero.

Top and Bottom Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical sides. Top and bottom refer to sides on plan view of bioretention.

Left Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical sides. Left refers to left side on plan view of bioretention.

Right Side Slope (ft/ft): H/V ratio of horizontal distance to vertical; 0 (zero) for vertical sides. Right refers to right side on plan view of bioretention.

Underdrain Diameter (in): This represents the diameter of the underdrain pipe. This does not include the storage capacity of the underdrain system.

Underdrain Orifice (in): To control the outflow from the underdrain it is possible to include an orifice. If you do not wish to have an orifice, then make the orifice diameter equal to the underdrain diameter.

Infiltration Rate (inches per hour): infiltration rate of the engineered soil for all layers.

Layer Depth (feet): depth of engineered soil.

Note that there can be a maximum of three different engineered soil layers.

Infiltration to the native soil can be turned on by setting Native Infiltration to YES. The parameters for native soil infiltration are:

Measured Infiltration Rate (inches per hour): infiltration rate of the native soil.


Infiltration Reduction Factor: between 0 and 1 (1/Native soil infiltration rate safety factor (see page 123)).

Use Wetted Surface Area (sidewalls): YES or NO; YES allows infiltration to the native soil through the sidewalls of the bioretention unit; otherwise all infiltration is through the bottom only.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

The user has two bioretention surface outlet configuration choices: (1) riser outlet structure, or (2) vertical orifice + overflow.

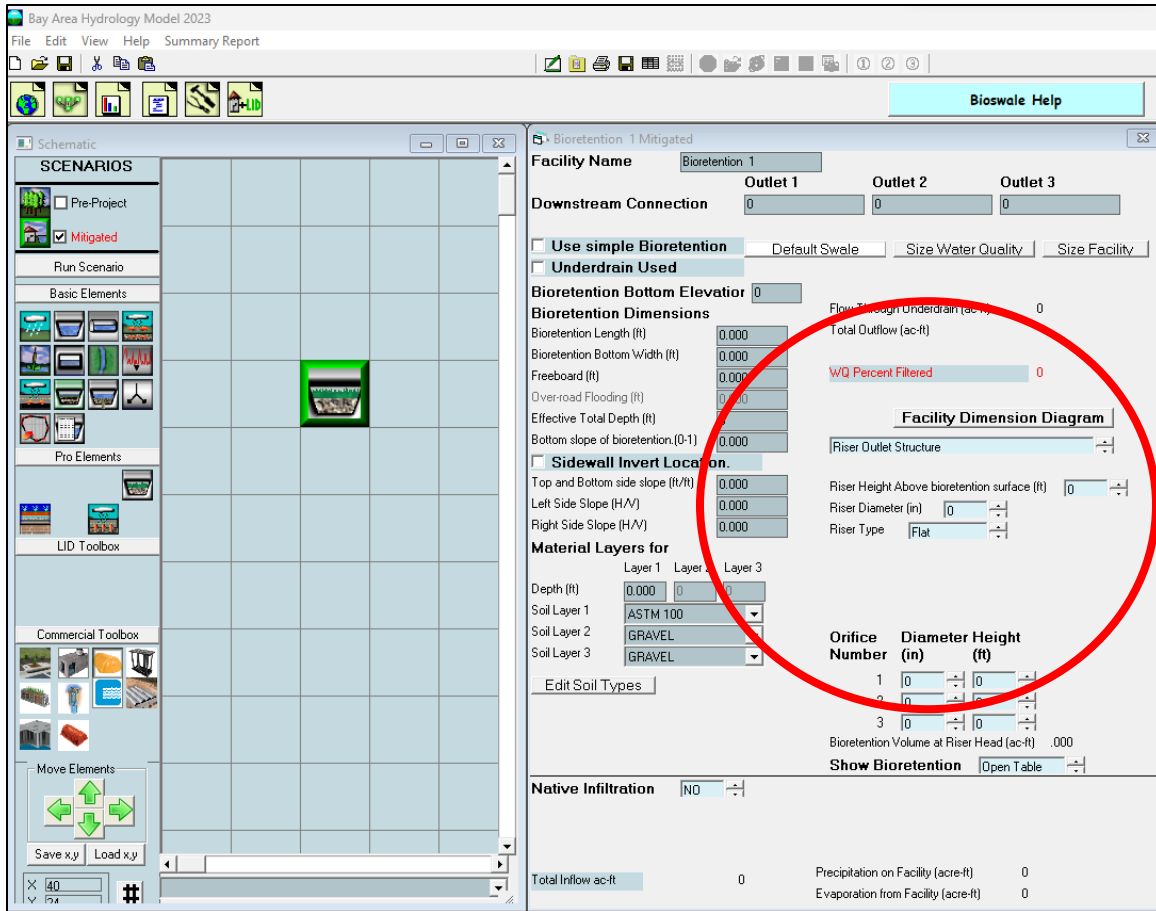

The input information required for the riser outlet structure is:

Riser Height above Bioretention (feet): depth of surface ponding before the riser is overtopped.

Riser Diameter (inches): diameter of the stand pipe.

Riser Type: Flat or Notched.


Notch Type: Rectangular, V-Notch, or Sutro.

For a rectangular notch:

Notch Height (feet): distance from the top of the weir to the bottom of the notch.

Notch Width (feet): width of notch; cannot be larger than the riser circumference.

For more information on riser notch options and orifices see discussion in OUTLET STRUCTURE CONFIGURATIONS section.

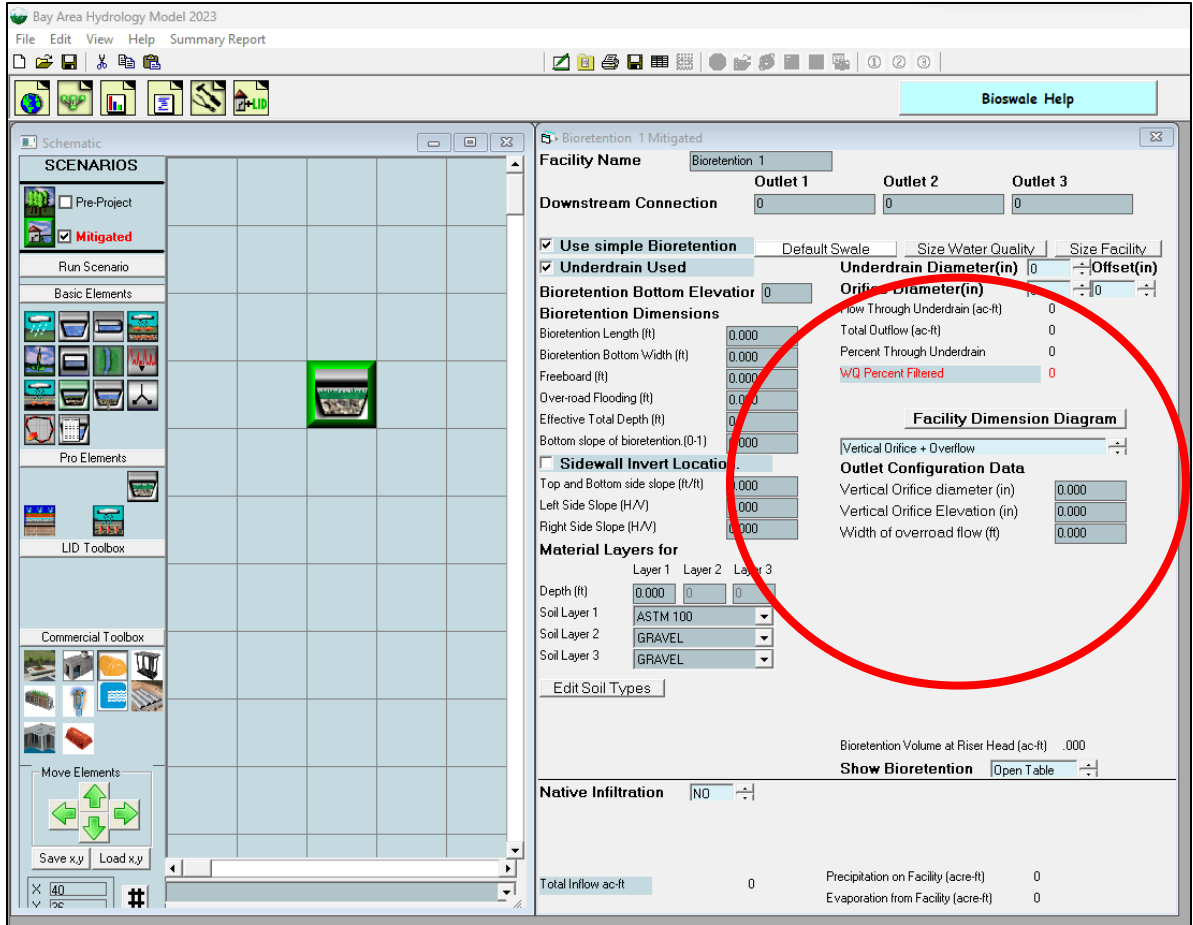

The input information required for the vertical orifice plus overflow is:


Vertical Orifice Diameter (inches): diameter of vertical opening below the weir.

Vertical Orifice Elevation (inches): vertical distance from the top of the engineered soil surface to the bottom of the vertical orifice.

Width of Over-road Flow (feet): weir/street length.


Over-road Flooding (ft): maximum depth of flow over weir/street (only required for vertical orifice plus overflow outlet).

Diagram of bioretention facility with vertical orifice plus overflow:

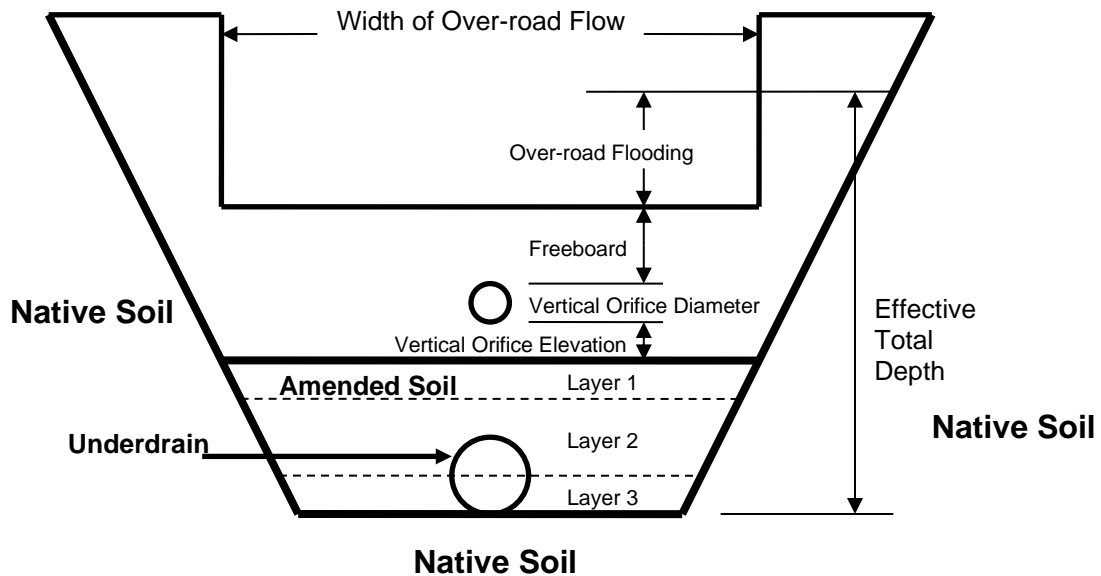

The bioretention element models a depression filled with one to three layers of amended soil. The amended soil layers provide Runoff Treatment by filtering the runoff. It can also have one or more surface outlets represented by an outlet structure with a riser and multiple orifices, or a vertical orifice and weir overflow structure.

The material layers represent the amended soils and their design characteristics (thickness and vertical water movement). These are the engineered soil layers added to the bioretention facility to filter the runoff prior to dispersal.

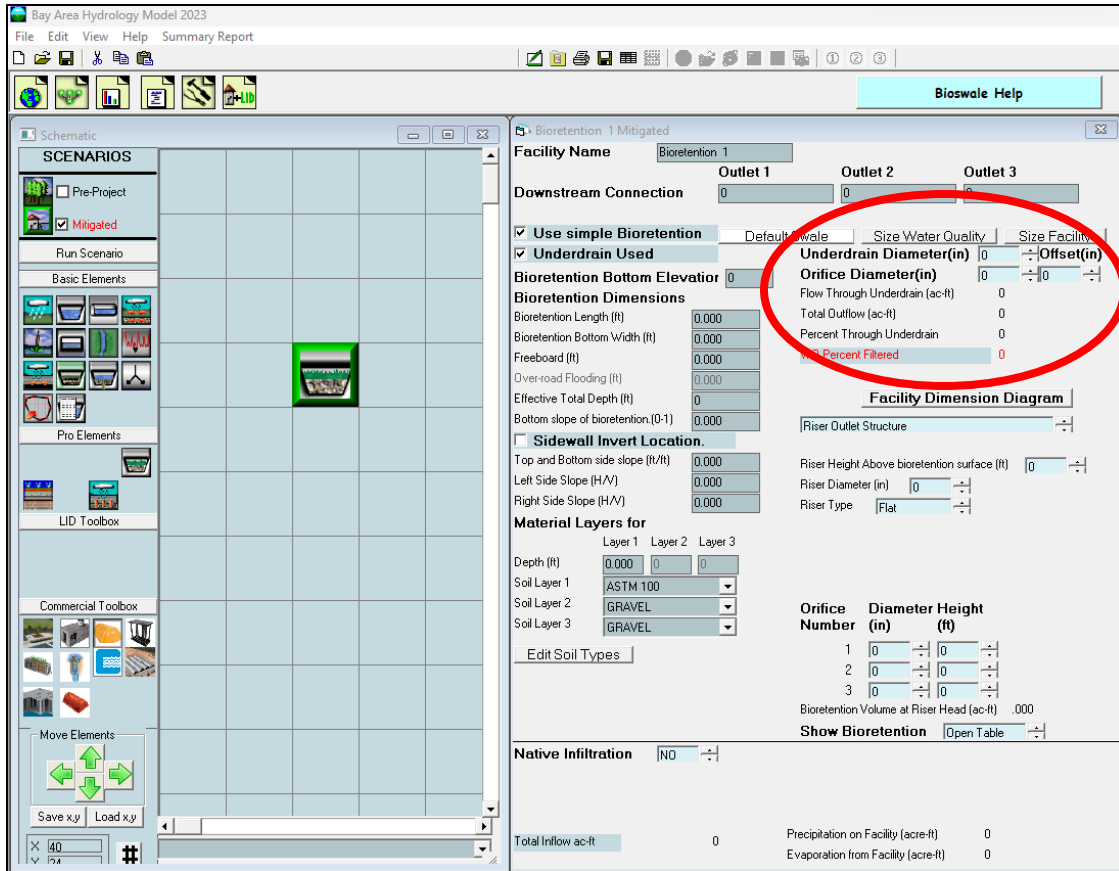

To use the underdrain, click the Underdrain Used box and input an underdrain diameter (inches) and the underdrain orifice diameter (inches). The bottom of the underdrain pipe is set by the user based on the offset (inches) above the bottom of the lowest engineered soil layer.

Underdrain Used: if C or D soil

Underdrain Diameter (in): Underdrain pipe diameter (set to zero if no underdrain is included).

Underdrain Orifice Diameter (in): underdrain pipe orifice opening diameter (set to zero if no underdrain is included; if you do not wish to have an orifice, then make the orifice diameter equal to the underdrain diameter).

The engineered soil layer fills with stormwater from the top on down to where it can drain to the native soil (if Native Infiltration is set to YES) and/or the underdrain pipe (if Underdrain Used box is checked). Water enters the underdrain when the engineered soil becomes saturated down to the top of the underdrain. The underdrain pipe fills and conveys water proportionally to the depth of engineered soil saturation. When the engineered soil is fully saturated, the underdrain pipe is at full capacity.

If native infiltration is turned on, then native infiltration will start when/if:

1. Water starts to fill the underdrain (if an underdrain is used).

2. Water enters the engineered soil (if Use Wetted Surface Area (sidewalls) is set to YES).
3. Water saturates the engineered soil layer(s) to two thirds of the total engineered soil depth (if there is no underdrain and Wetted Surface Area is set to NO).

Determine rectangular shape from irregular shaped bioretention.

Method for calculating rectangular shape:

1. Compute surface area at bottom.
2. Compute surface area at top.
3. Take square root of bottom surface area.
4. Take square root of top surface area.
5. Compute surface at 1-foot intervals.
6. Take square root at 1-foot intervals.

An example bioretention table can be seen down below:


Height above bottom (ft)	Surface Area (sq-ft)	Length (ft)	Width (ft)	Side Slope	Description
0	1000	31.62	31.62	1.54	Incremental Side Slope
1	1100	33.17	33.17	1.48	
2	1200	34.64	34.64	1.42	
3	1300	36.06	36.06	1.36	
4	1400	37.42	37.42	1.31	
5	1500	38.73	38.73	1.27	
6	1600	40.00	40.00	1.23	
7	1700	41.23	41.23	1.37	Average Side Slope

In this example, if you know the surface area only at zero feet and 7 feet above the bottom of the bioretention then use the calculated average side slope (in this example it is 1.37 H:V) for all four side slopes.

Learn more about the Bioretention element here:
www.clearcreeksolutions.info/bahm-course-home

IN-GROUND (INFILTRATION) PLANTER ELEMENT


An in-ground planter allows stormwater to enter the planter above ground and then infiltrate through the soil and gravel storage layers before exiting through a discharge pipe. Water can also infiltrate into the native soil beneath the planter.

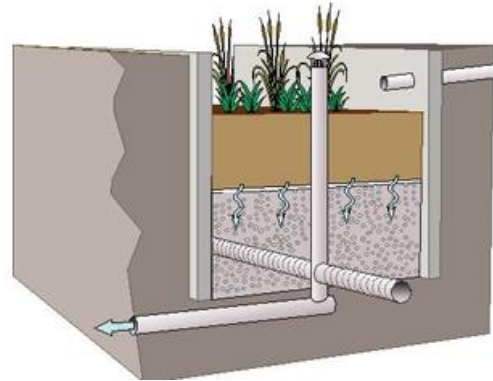

In-Ground (Infiltration) Planter

For the purpose of flow control, the discharge from the pipe should not exceed the pre-project discharge from the project site for the flow duration range specified by the local jurisdiction.

In BAHM2023, the in-ground planter is represented by a specialized application of the bioretention element available in the LID Toolbox. To access the elements in the LID Toolbox menu, click on the LID Toolbox bar.

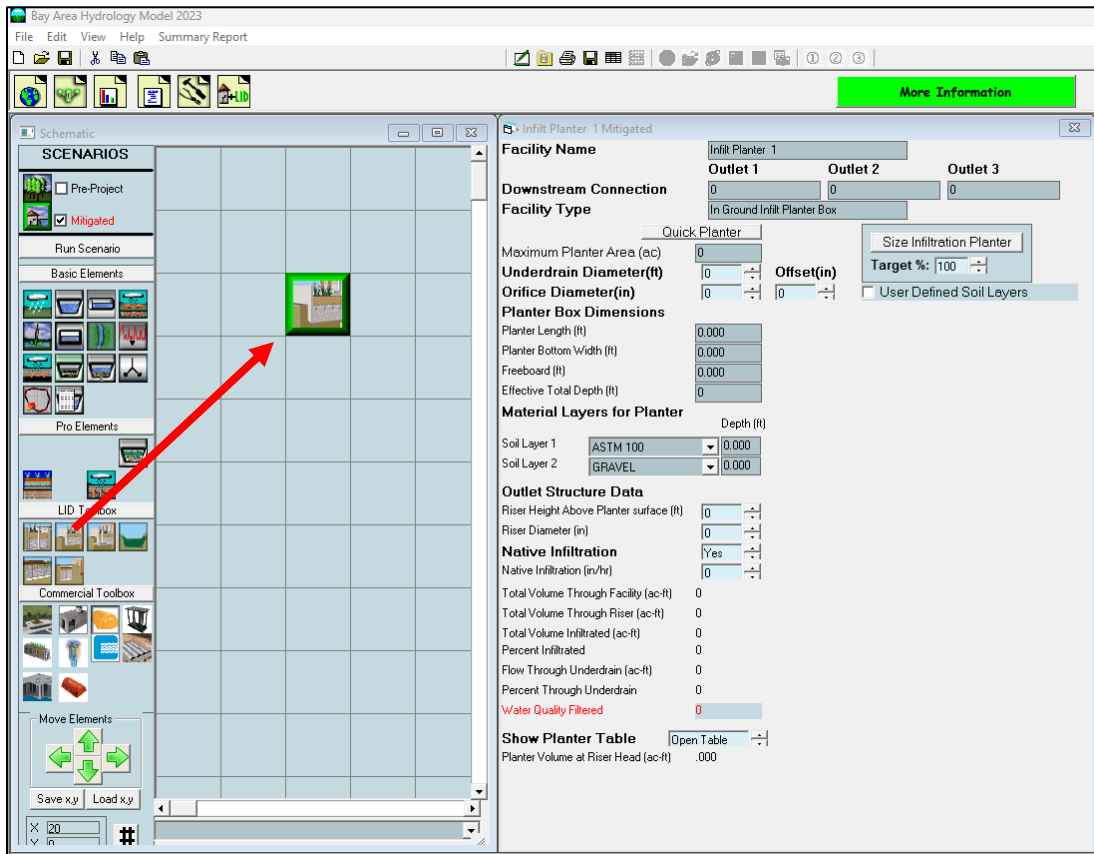

The in-ground (infiltration) planter dimensions and parameters are:

Planter Length (ft): Length of planter box.

Planter Bottom Width (ft): Width of planter box.

Freeboard: Additional storage height above top of riser.

Effective Total Depth (ft): Planter height from bottom of planter to top of riser plus freeboard.

Soil Layer 1 Type: Select from Soil Type pulldown menu (select BAHM 5).

Soil Layer 1 (ft): Planter soil layer depth.

NOTE: All bioretention-type facilities used in the Bay Area must use the biotreatment soil mix specified in the Municipal Regional Stormwater Permit (MRP) for the top layer (see “Revised Model Biotreatment Soil Media Specifications”, BASMAA, 2016 for more details). This biotreatment soil mix is represented by “BAHM 5”, which contains the appropriate soil values to meet the specification.

The first engineered soil layer should be the BAHM 5 soil mix specified by the Municipal Regional Stormwater Permit.

Soil Layer 2 Type: Select from Soil Type pulldown menu (usually gravel).

Soil Layer 2 (ft): Planter gravel layer depth.

To use an underdrain, click the Underdrain Used box and input an underdrain diameter (inches) and the underdrain orifice diameter (inches). The bottom of the underdrain pipe is set by the user based on the offset (inches) above the bottom of the lowest engineered soil layer.

Underdrain Used: if C or D soil

Underdrain Diameter (in): Planter underdrain pipe diameter (set to zero if no underdrain is included).

Orifice Diameter (in): Planter underdrain pipe orifice diameter (set to zero if no underdrain is included; if you do not wish to have an orifice, then make the orifice diameter equal to the underdrain diameter).

Riser Height Above Planter Surface (ft): Height of planter overflow pipe above planter soil surface.


Riser Diameter (in): Planter overflow pipe diameter.

Native Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

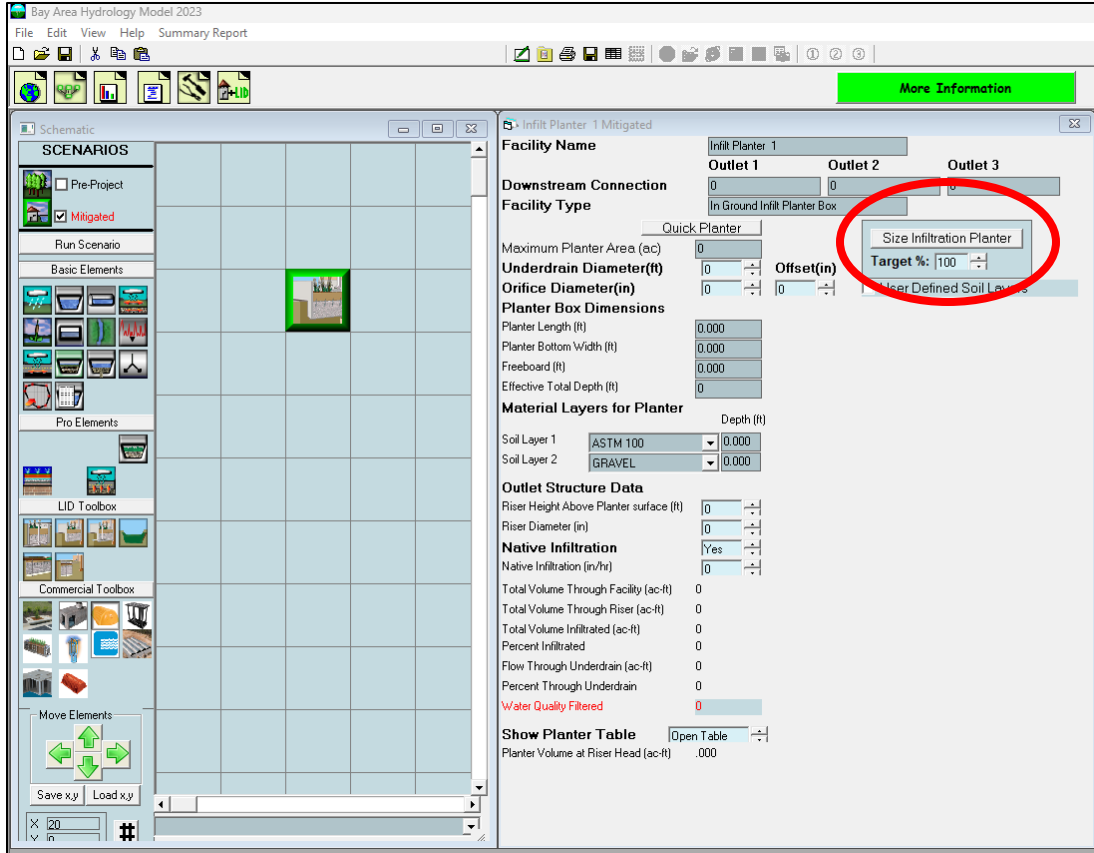


BAHM2023 includes automated sizing of the planter box (“Quick Planter”) based on a user-set target infiltration percentage. After the target percentage is set then the user can click on the Size Infiltration Planter button. BAHM2023 will iterate to determine the planter length and width needed to meet the target infiltration percentage.

Learn more about the In-Ground Planter Element element here:
www.clearcreeksolutions.info/bahm-course-home


FLOW-THROUGH PLANTER ELEMENT

A flow-through planter is similar to the in-ground (infiltration) planter, except that water is not allowed to infiltrate into the native soil underlying the gravel layer of the planter. As with the in-ground planter, stormwater enters the planter above ground and then infiltrate through the soil and gravel storage layers before exiting through a discharge pipe.

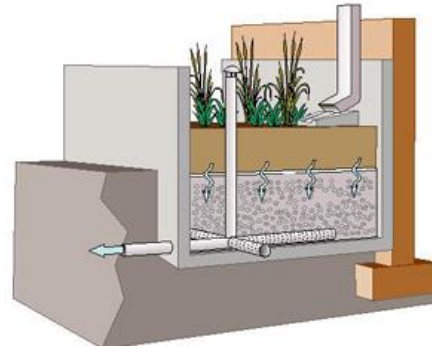

For the purpose of flow control the discharge from the pipe should not exceed the pre-project discharge from the project site for the flow duration range specified by the local jurisdiction.

In BAHM2023 the flow-through planter is represented by a specialized application of the bioretention element available in the LID Toolbox. To access the elements in the LID Toolbox menu click on the LID Toolbox bar.

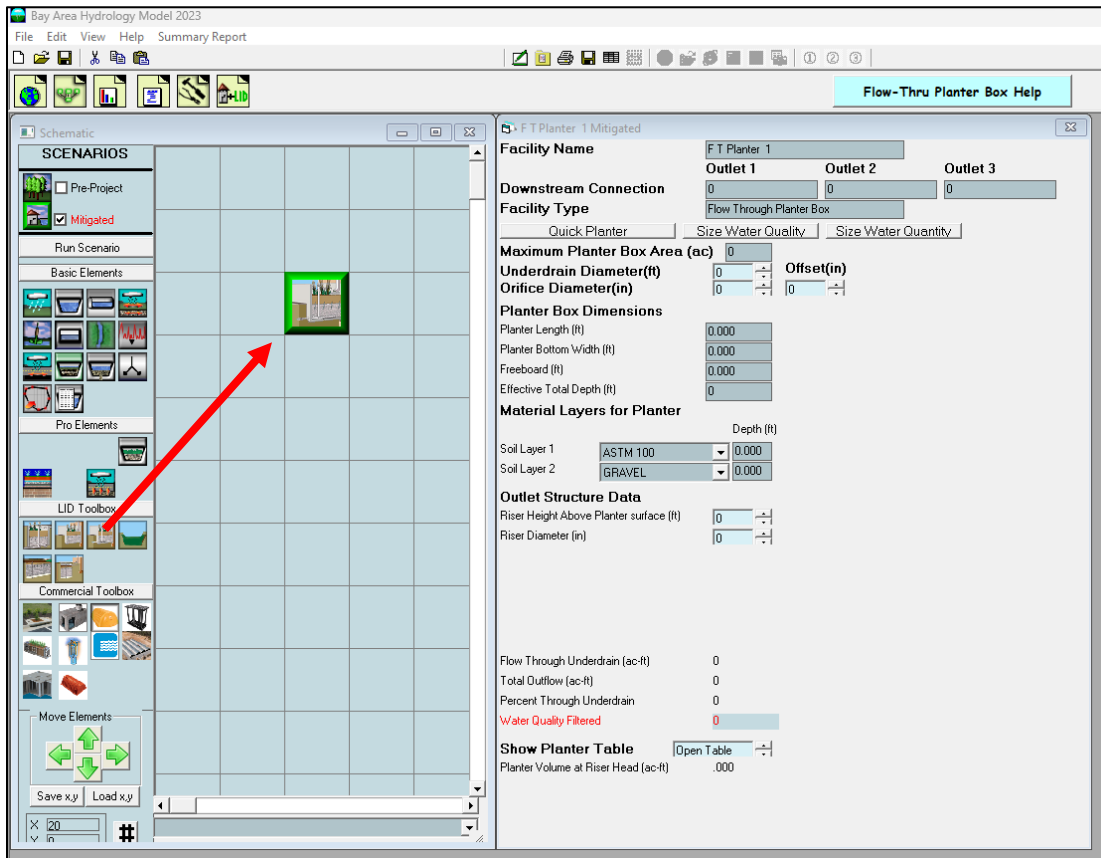

The flow-through planter dimensions and parameters are:

Planter Length (ft): Length of planter box.

Planter Bottom Width (ft): Width of planter box.

Freeboard: Additional storage height above top of riser.

Effective Total Depth (ft): Planter height from bottom of planter to top of riser plus freeboard.

Soil Layer 1 Type: Select from Soil Type pulldown menu (select BAHM 5).

Soil Layer 1 (ft): Planter soil layer depth.

NOTE: All bioretention-type facilities used in the Bay Area must use the biotreatment soil mix specified in the Municipal Regional Stormwater Permit (MRP) for the top layer (see “Revised Model Biotreatment Soil Media Specifications”, BASMAA, 2016 for more details). This biotreatment soil mix is represented by “BAHM 5”, which contains the appropriate soil values to meet the specification.

The first engineered soil layer should be the BAHM 5 soil mix specified by the Municipal Regional Stormwater Permit.

Soil Layer 2 Type: Select from Soil Type pulldown menu (usually gravel).

Soil Layer 2 (ft): Planter gravel layer depth.

Since no infiltration into native soil is allowed in a flow-through planter, an underdrain is required. The underdrain pipe should be set at the bottom of the planter, so the offset (height above the bottom of the lowest engineered soil layer) should be set to zero.

Underdrain Diameter (in): Planter underdrain pipe diameter.

Orifice Diameter (in): Planter underdrain pipe orifice diameter (if you do not wish to have an orifice, then make the orifice diameter equal to the underdrain diameter).

Riser Height Above Planter Surface (ft): Height of planter overflow pipe above planter soil surface.

Riser Diameter (in): Planter overflow pipe diameter.

The only difference between an in-ground (infiltration) planter and a flow-through planter is whether or not native infiltration is allowed.

Learn more about the Flow Through Planter element here:
www.clearcreeksolutions.info/bahm-course-home


PERMEABLE PAVEMENT ELEMENT

Permeable pavement LID options include porous asphalt or concrete and grid/lattice systems (non-concrete) and paving blocks. The use of any of these LID options requires that certain minimum standards and requirements are met related to subgrade, geotextile material, separation or bottom filter layer, base material, wearing layer, drainage conveyance, acceptance testing, and surface maintenance.

NOTE: Permeable pavement can be used in place of conventional pavement for roadways, sidewalks, driveways, and parking lots. Check with the local municipal permitting agency to find out under what conditions permeable pavement is allowed.

Permeable pavement can be represented by the permeable pavement element in BAHM2023 if the following three conditions are met:

1. The infiltration rate of the permeable pavement is greater than the peak rainfall rate.
2. The infiltration rate of the permeable pavement is greater than the underlying native soil.
3. There is subgrade layer of crushed rock/gravel between the permeable pavement and the native soil.

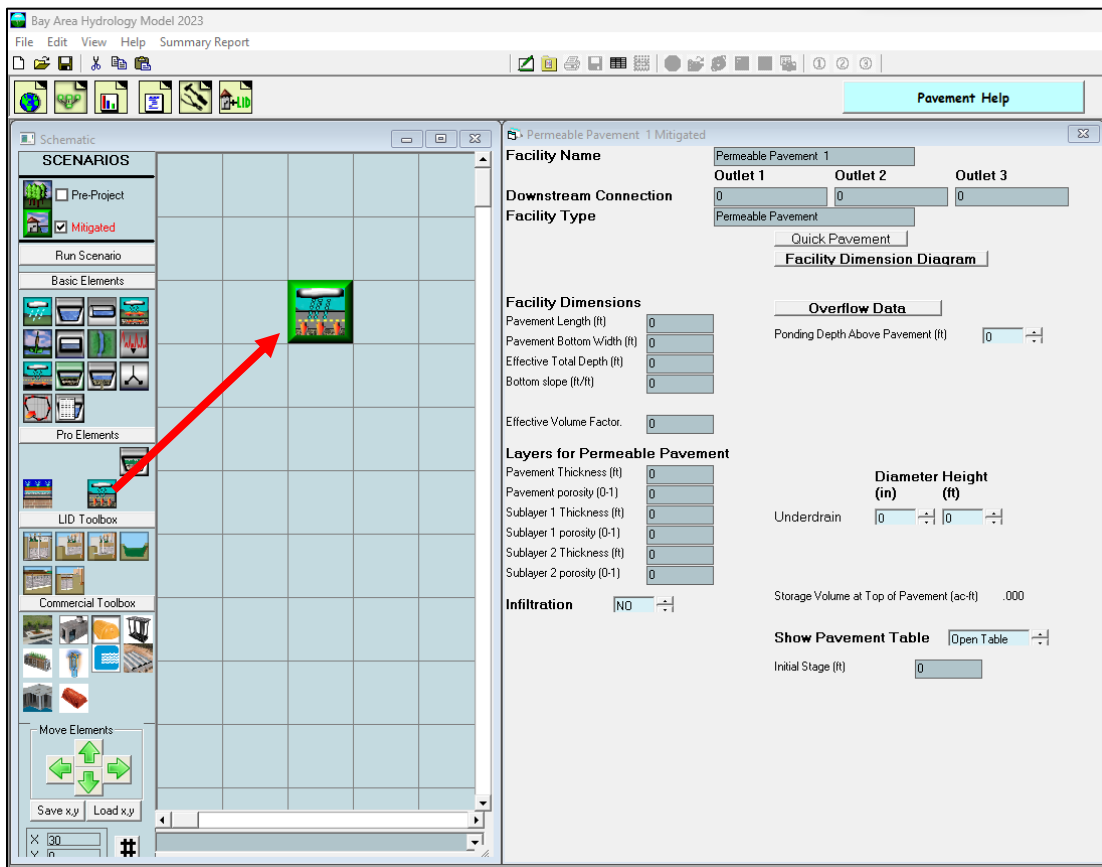

The permeable pavement element (also called porous pavement) is an impervious basin element that drains directly to storage layer similar to a gravel trench bed.

Outlet 1: Control structure discharge (i.e., for permeable pavement, surface flow and underdrain discharge).

Outlet 2: Infiltration.

Outlet 3: Not used.

The permeable pavement element dimensions and parameters are:

Pavement Length (ft): Roadway length.

Pavement Bottom Width (ft): Roadway width.

Effective Total Depth (ft): Height from bottom of permeable pavement subgrade to top of pavement plus at least 0.5 feet extra.

Bottom Slope (ft/ft): Gravel layer slope or grade.

The effective volume factor is a value between zero and 1.00. It is only used when the bottom slope is greater than 2%. The effective volume factor is the fraction ratio of the average maximum water depth behind a check dam in the gravel layer (Sublayer 1) compared to the maximum gravel layer depth (Sublayer 1). For example, if the average maximum water height is 6" and the gravel depth is 9" then the Effective Volume Factor = 0.67 (6/9). The effective volume factor is multiplied by the Sublayer 1 storage volume to determine the actual maximum volume available for stormwater storage before the check dam is overtopped and the water in the gravel layer depth (Sublayer 1) proceeds to a downstream conveyance facility.

Pavement Thickness (ft): Permeable pavement layer depth.

Pavement Porosity: Permeable pavement porosity.

Layer 1 Thickness (ft): Subgrade gravel layer depth.

Layer 1 Porosity: Subgrade gravel porosity.

Layer 2 Thickness (ft): Sand layer depth (if appropriate).

Layer 2 Porosity: Sand porosity.

Ponding Depth Above Pavement (ft): Height at which sheet flow occurs on the pavement.

Underdrain Diameter (in): Set to zero if there is no underdrain.

Underdrain Height (ft): Height of the bottom of the underdrain above the bottom layer.

Native Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

Infiltration Reduction Factor: 1/Native soil infiltration rate safety factor (see page 123).

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

The permeable pavement layers represent the pavement layer and two subgrade layers and their design characteristics (thickness and porosity). The subgrade layers (Sublayer 1 and Sublayer 2) are available to provide storage prior to discharge through infiltration to the native soil or discharge via an underdrain.

Quick Pavement will create a permeable pavement feature with default values without checking it for compliancy with flow duration standards.

The permeable pavement surface area automatically receives rainfall and produces evapotranspiration. Due to this model input, the permeable pavement surface area should be excluded from the basin element's total surface area.

NOTE: Check with Appendix D or the local municipal permitting agency to find out if ponding on the surface of the pavement is allowed.

If ponding is not allowed, then the ponding depth above pavement value should be set to zero.


Learn more about the Permeable Pavement element here:
www.clearcreeksolutions.info/bahm-course-home


DISPERSION

LID Dispersion practices can include roof runoff dispersion onto adjacent yard area, parking lot runoff onto adjacent lawn area, and reverse slope sidewalks draining onto adjacent vegetated areas.

NOTE: Specific minimum requirements and standards must be met to allow dispersion (see the local municipal permitting agency for details).

Dispersion is represented in BAHM2023 with lateral flow basin elements.

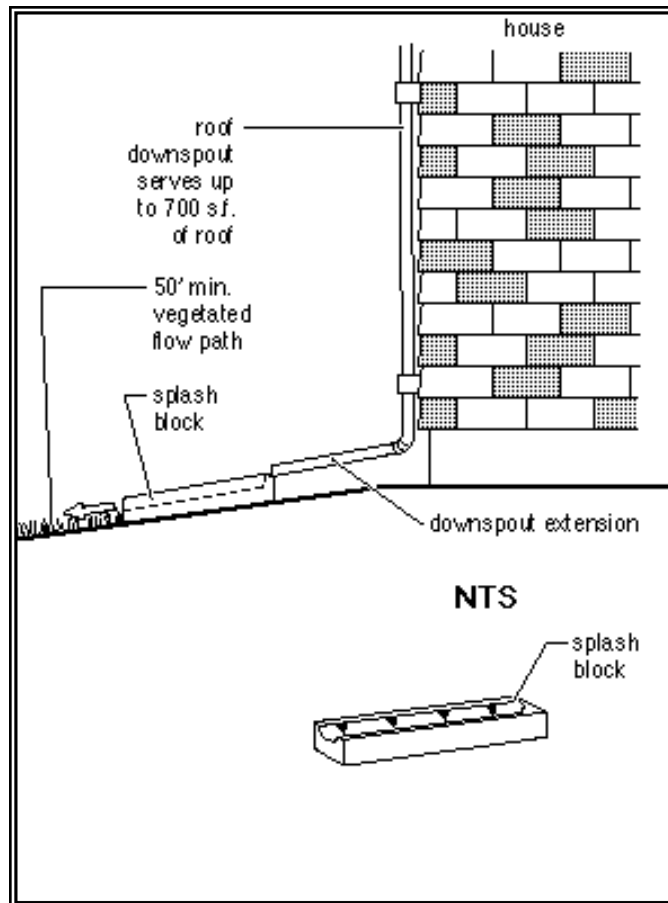

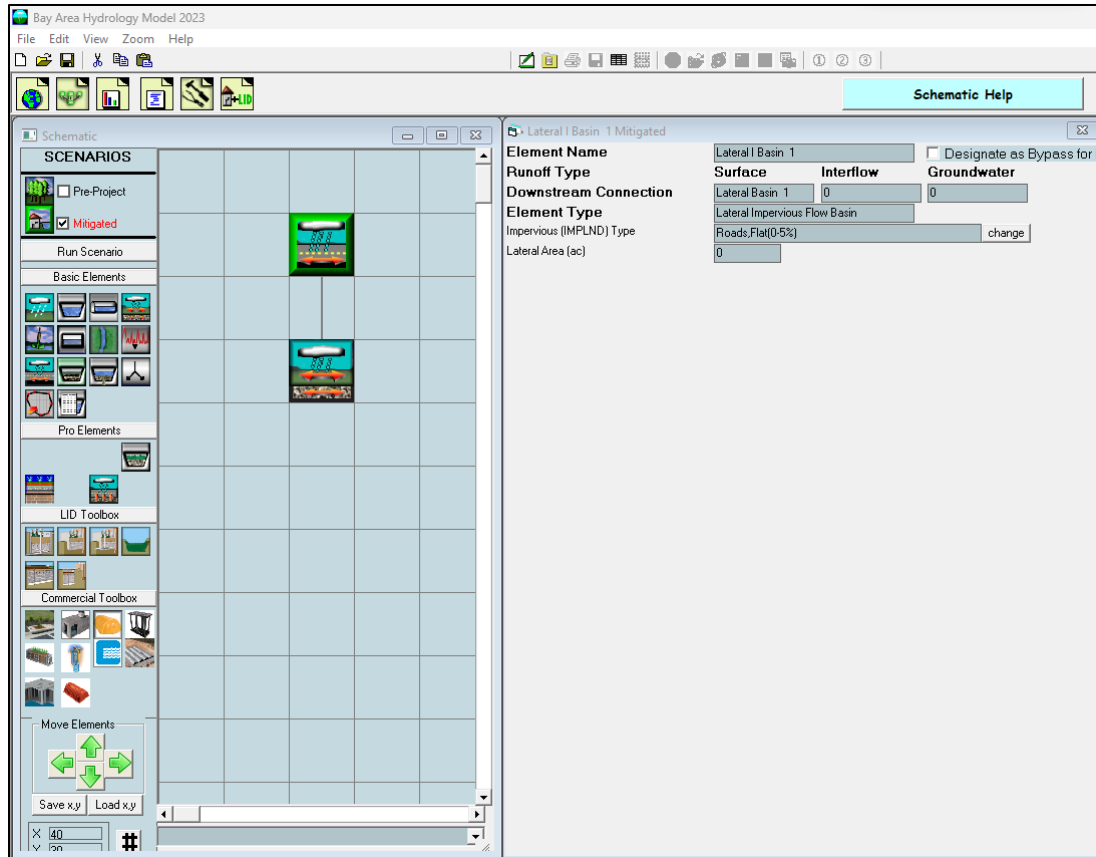

Roof Dispersion Runoff Example


The impervious lateral basin (Lateral I Basin 1 in the above scenario) is connected to the pervious lateral basin (Lateral Basin 1). All of the runoff generated by impervious roof Lateral I Basin 1 is distributed onto pervious urban Lateral Basin 1 before routing to a stormwater control facility (pond, vault, etc.).

The lateral basin dimensions and parameters to adjust to represent dispersion are:

Impervious/IMPLND type: select either road, roof, sidewalks, parking, or driveways and the associated slope category (all roofs are the same; there is no roof slope category).

Soil (PERLND) type: select one of the 48 different pervious land types based on soil, vegetation, and slope. A and B soils will provide more dispersion benefits than C or D soils because of their ability to infiltrate more runoff.


Lateral Area: size of contributing or receiving area (acres).

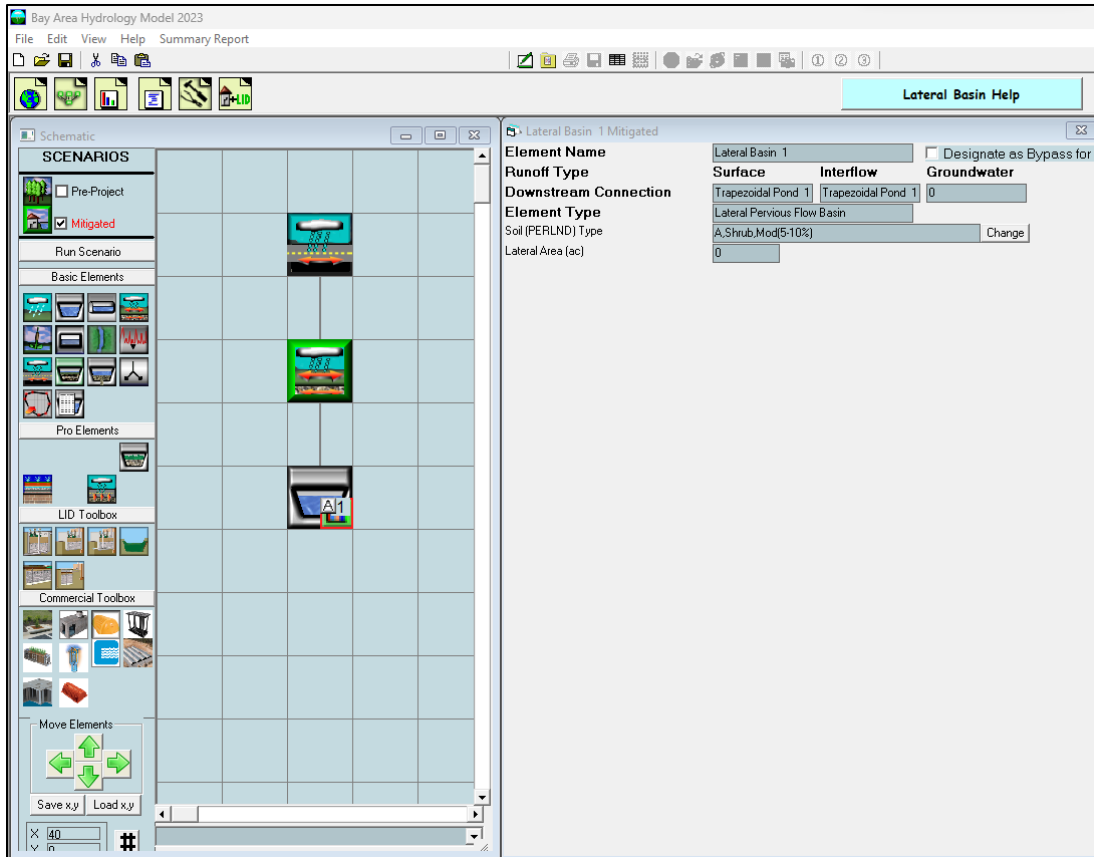

Dispersion will decrease the total runoff, but will not totally eliminate the need for a stormwater control facility. A pond can be connected to the discharge from the pervious lateral basin to provide the final required mitigation.

Learn more about Dispersion here:
www.clearcreeksolutions.info/bahm-course-home

LATERAL SOIL BASIN ELEMENT (Pervious)

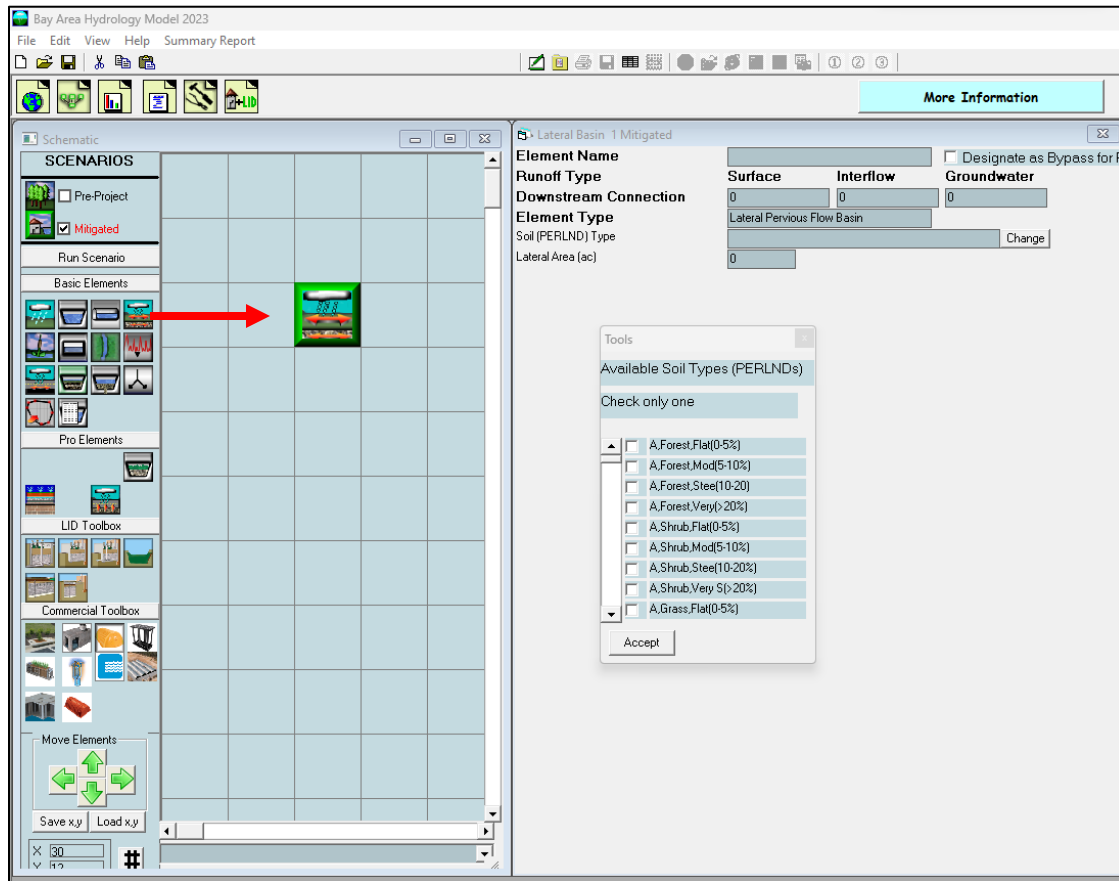

Runoff dispersion from impervious surfaces onto adjacent pervious land can be modeled using pervious and impervious lateral basins. For example, runoff from an impervious parking lot can sheet flow onto an adjacent lawn prior to draining into a stormwater conveyance system. This action slows the runoff and allows for some limited infiltration into the pervious lawn soil prior to discharging into a conveyance system.


The pervious lateral basin is similar to the standard basin except that the runoff from the lateral basin goes to another adjacent lateral basin (impervious or pervious) rather than directly to a conveyance system or stormwater facility. By definition, the pervious lateral basin contains only a single pervious land type. Impervious area is handled separately with the impervious lateral basin (Lateral I Basin).

The user selects the pervious lateral basin land type by checking the appropriate box on the Available Soil Types Tools screen. This information is automatically placed in the Soil (PERLND) Type box above. Once entered, the land type can be changed by clicking on the Change button on the right.

The user enters the number of acres represented by the lateral soil basin land type. If the lateral basin contains two or more pervious land use types, then the user should create a separate lateral basin for each.

Learn more about the Lateral Pervious Basin element here:
www.clearcreeksolutions.info/bahm-course-home

LATERAL IMPERVIOUS AREA ELEMENT (Impervious)

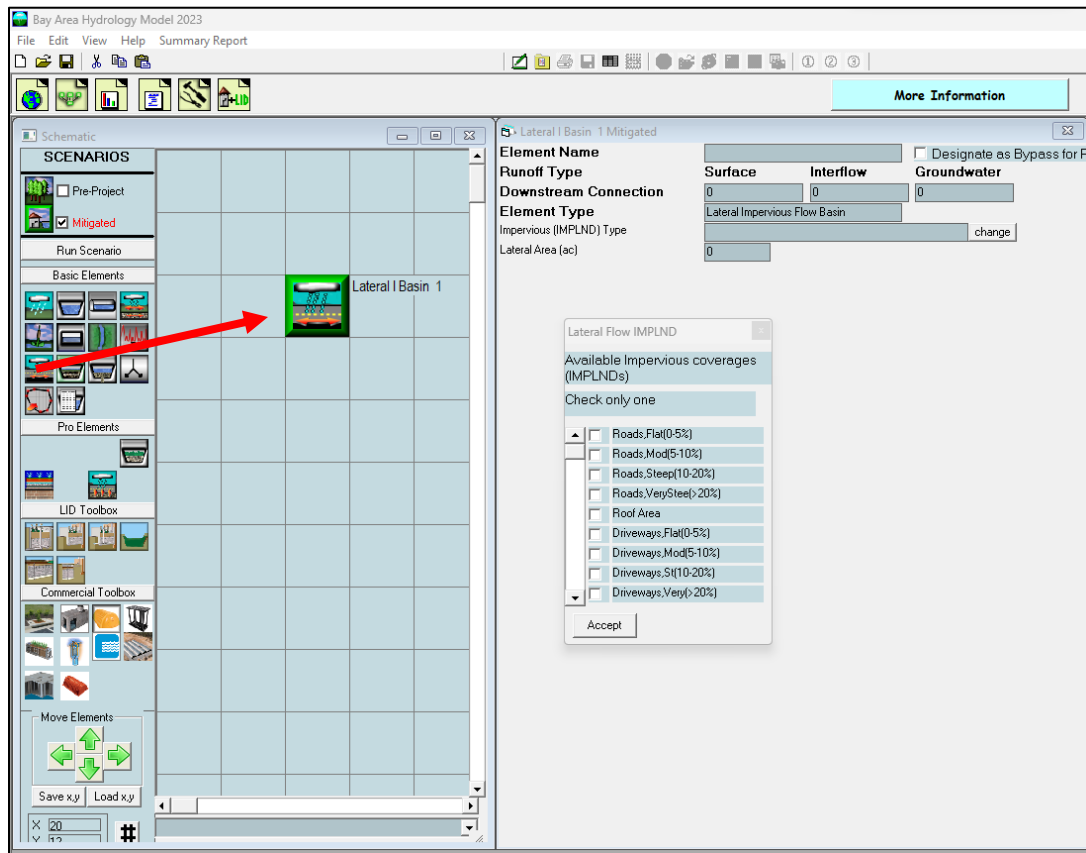

The impervious lateral basin is similar to the standard basin except that the surface runoff from the lateral impervious basin goes to another adjacent lateral basin (impervious or pervious) rather than directly to a conveyance system or stormwater facility. By definition, the impervious lateral basin contains only impervious land types. Pervious area is handled separately with the pervious lateral basin (Lateral Soil Basin).


The user selects the impervious lateral basin land type by checking the appropriate box on the Available Impervious Coverages screen. This information is automatically placed in the Impervious (IMPLND) Type box above. Once entered, the land type can be changed by clicking on the Change button on the right.

The user enters the number of acres represented by the lateral impervious basin land type. If the lateral impervious basin contains two or more impervious land use types, then the user should create a separate lateral impervious area basin for each.


For example, to model parking lot runoff dispersion onto adjacent lawn, connect the Lateral Impervious Area (the parking lot) to the Lateral Soil Basin (the lawn). In the model's calculations, surface runoff from the parking lot is added to the surface of the lawn (urban vegetation). The total runoff will then be directed to a stormwater conveyance system as defined by the user.

DRY WELL ELEMENT

A dry well is similar to the in-ground (infiltration) planter, except that there is no bottom discharge pipe or underdrain. Water must infiltrate into the native soil underlying the gravel layer of the planter. The native soil must have sufficient infiltration capacity to infiltrate all of the stormwater.

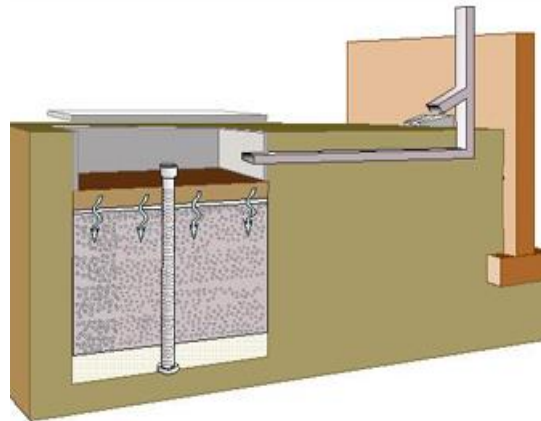

In BAHM2023, the dry well is represented by a specialized application of the gravel trench element available in the LID Toolbox. To access the elements in the LID Toolbox menu, click on the LID Toolbox bar.

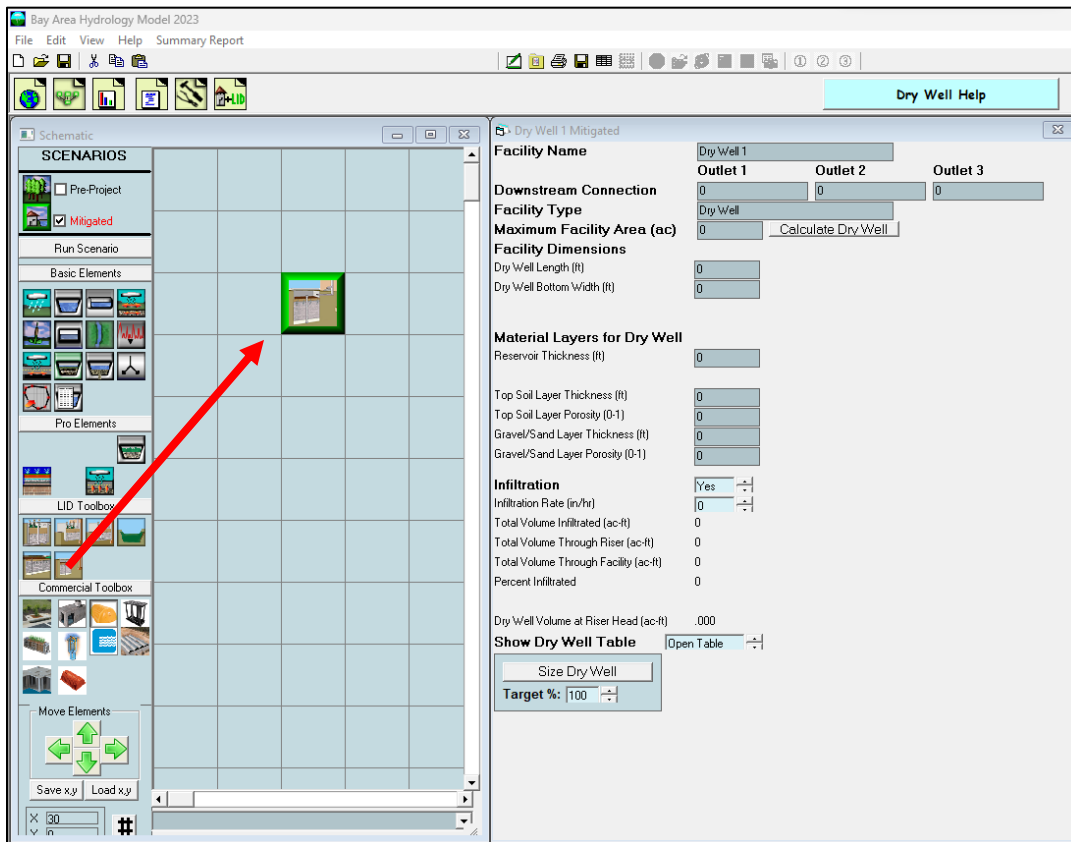

The dry well dimensions and parameters:

Dry Well Length (ft): Length of well.

Dry Well Width (ft): Width of well.

Reservoir Thickness (ft): Depth of open water storage.

Top Soil Layer Thickness (ft): Dry well soil layer depth.

Top Soil Layer Porosity: Dry well soil porosity.

Gravel/Sand Layer Thickness (ft): Dry well gravel layer depth.

Gravel/Sand Layer Porosity: Dry well gravel porosity.

Native Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

BAHM2023 includes automated sizing of the dry well based on a user-set target infiltration percentage. After the target percentage is set, then the user can click on the Size Dry Well button. BAHM2023 will iterate to determine the dry well length and width needed to meet the target infiltration percentage.


NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

Note that the dry well is covered; there is no precipitation on or evaporation from the dry well.


Learn more about the Dry Well element here:
www.clearcreeksolutions.info/bahm-course-home

INFILTRATION TRENCH ELEMENT

An infiltration trench is similar to the dry well. There is no bottom discharge pipe or underdrain. Water must infiltrate into the native soil underlying the gravel layer of the planter. The native soil must have sufficient infiltration capacity to infiltrate all of the stormwater.

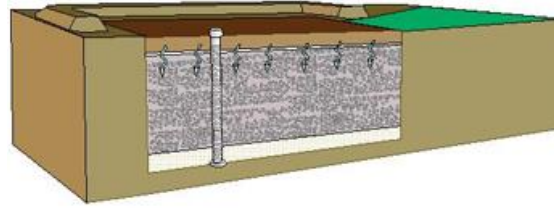

In BAHM2023, the infiltration trench is represented by a specialized application of the gravel trench element available in the LID Toolbox. To access the elements in the LID Toolbox menu click on the LID Toolbox bar.

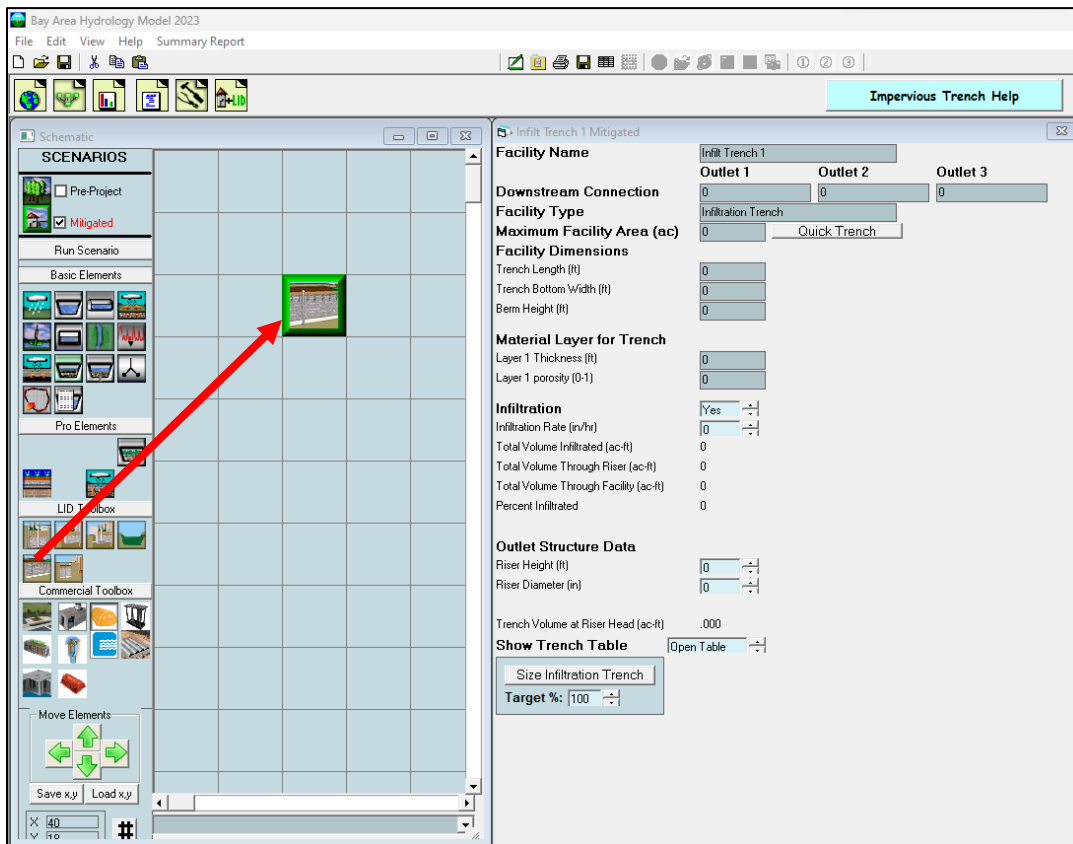

The infiltration trench dimensions and parameters are:

Trench Length (ft): Infiltration trench length.

Trench Bottom Width (ft): Infiltration trench width.

Berm Height (ft): Height above top of trench at which overflow occurs (one foot above riser height).

Layer 1 Thickness (ft): Infiltration trench soil layer depth.

Layer 1 Porosity: Infiltration trench soil porosity.

Riser Height (ft): Height of infiltration trench overflow pipe above trench soil surface. If a weir is preferred instead of a riser, then set the riser height to the weir height and set the riser diameter to the weir length.

Riser Diameter (in): Infiltration trench overflow pipe diameter.

Native Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

The infiltration trench does not include an underdrain. If an underdrain is required, then use the gravel trench element (page 59) instead and set the underdrain height and orifice diameter using the orifice input (the orifice height is defined as from the bottom of the lowest layer in the trench).

BAHM2023 includes automated sizing of the infiltration trench based on a user-set target infiltration percentage. After the target percentage is set, then the user can click on the Size Infiltration Trench button. BAHM2023 will iterate to determine the infiltration trench length and width needed to meet the target infiltration percentage.


NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

Note that, unlike the dry well, the infiltration trench receives precipitation on and evaporation from the trench surface.

Learn more about the Infiltration Trench element here:
www.clearcreeksolutions.info/bahm-course-home


INFILTRATION BASIN ELEMENT

An infiltration basin/pond allows stormwater to enter the basin/pond above ground and then infiltrate through the bottom of the basin/pond before exiting through a discharge pipe. Water can also infiltrate into the native soil beneath the basin/pond.

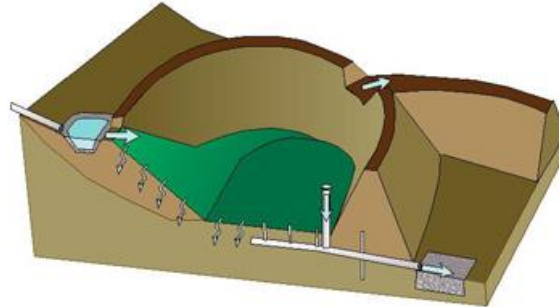

For the purpose of flow control the discharge from the pipe should not exceed the pre-project discharge from the project site for the flow duration range specified by the local jurisdiction.

In BAHM2023, the infiltration basin/pond is represented by a specialized application of the trapezoidal pond element available in the LID Toolbox. To access the elements in the LID Toolbox menu, click on the LID Toolbox bar.

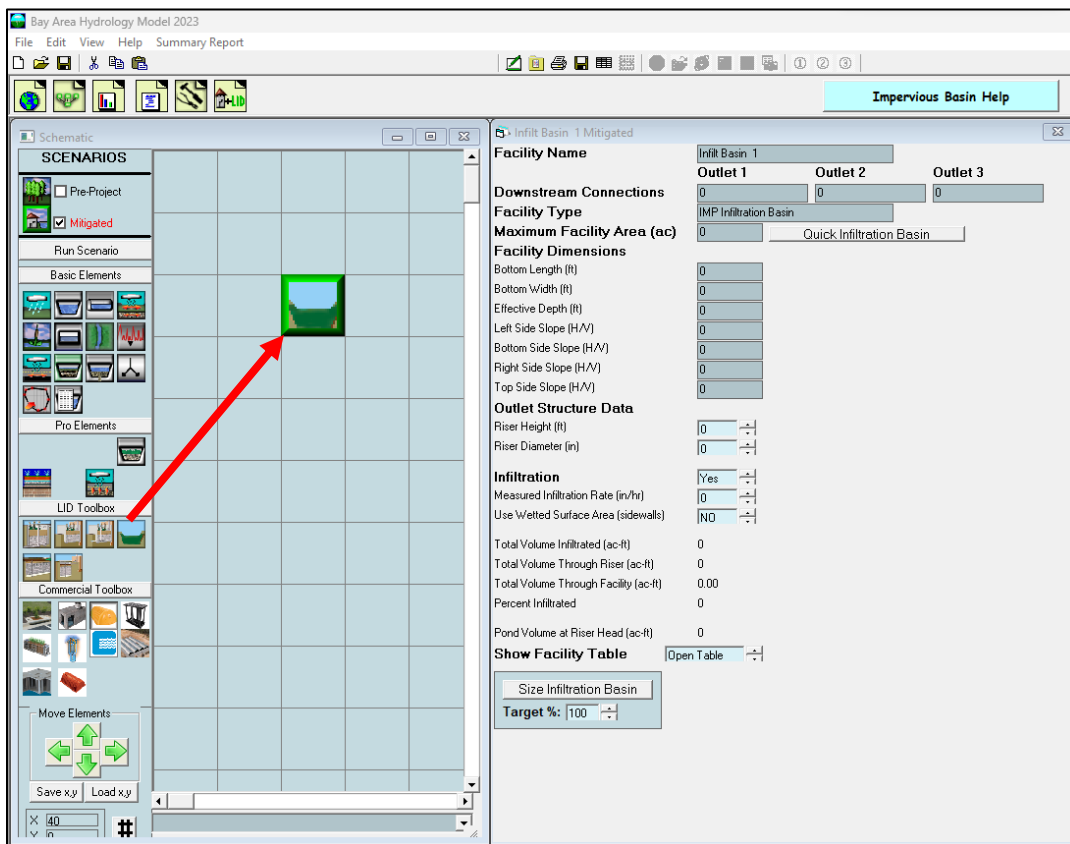

The infiltration basin/pond dimensions and parameters are:

Bottom Length (ft): Infiltration basin/pond length.

Bottom Width (ft): Infiltration basin/pond width.

Effective Depth (ft): Infiltration basin height from basin/pond bottom to top of riser plus at least 0.5 feet extra.

Left Side Slope (H/V): 0 (zero) for vertical infiltration basin/pond sides.

Bottom Side Slope (H/V): 0 (zero) for vertical infiltration basin/pond sides.

Right Side Slope (H/V): 0 (zero) for vertical infiltration basin/pond sides.

Top Side Slope (H/V): 0 (zero) for vertical infiltration basin/pond sides.

Riser Height (ft): Height of infiltration basin/pond overflow pipe above basin/pond soil surface.

Riser Diameter (in): Infiltration basin/pond overflow pipe diameter.

Infiltration: Yes (infiltration into the underlying native soil)

Measured Infiltration Rate (in/hr): Native soil infiltration rate.

Use Wetted Surface Area (sidewalls): Yes, if infiltration through the basin/pond side slopes is allowed.

If infiltration is used, then the user should consult the Infiltration discussion on page 123.

BAHM2023 includes automated sizing of the infiltration basin/pond based on a user-set target infiltration percentage. After the target percentage is set, then the user can click on the Size Infiltration Basin button. BAHM2023 will iterate to determine the infiltration basin/pond length and width needed to meet the target infiltration percentage.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.


An infiltration basin/pond receives precipitation on and evaporation from the basin/pond surface.

Learn more about the Permeable Pavement element here:
www.clearcreeksolutions.info/bahm-course-home


GREEN ROOF ELEMENT

A green roof is roof covered with vegetation and a growing medium (typically an engineered soil mix). Green roofs are not always green and are also known as vegetated roofs or eco-roofs.

The advantage of a green roof is its ability to store some runoff on the plants' surfaces and in the growing medium. Evapotranspiration by the plants and growing medium reduces the total runoff. Runoff movement through the growing medium slows down the runoff and reduces peak discharge during storm events.

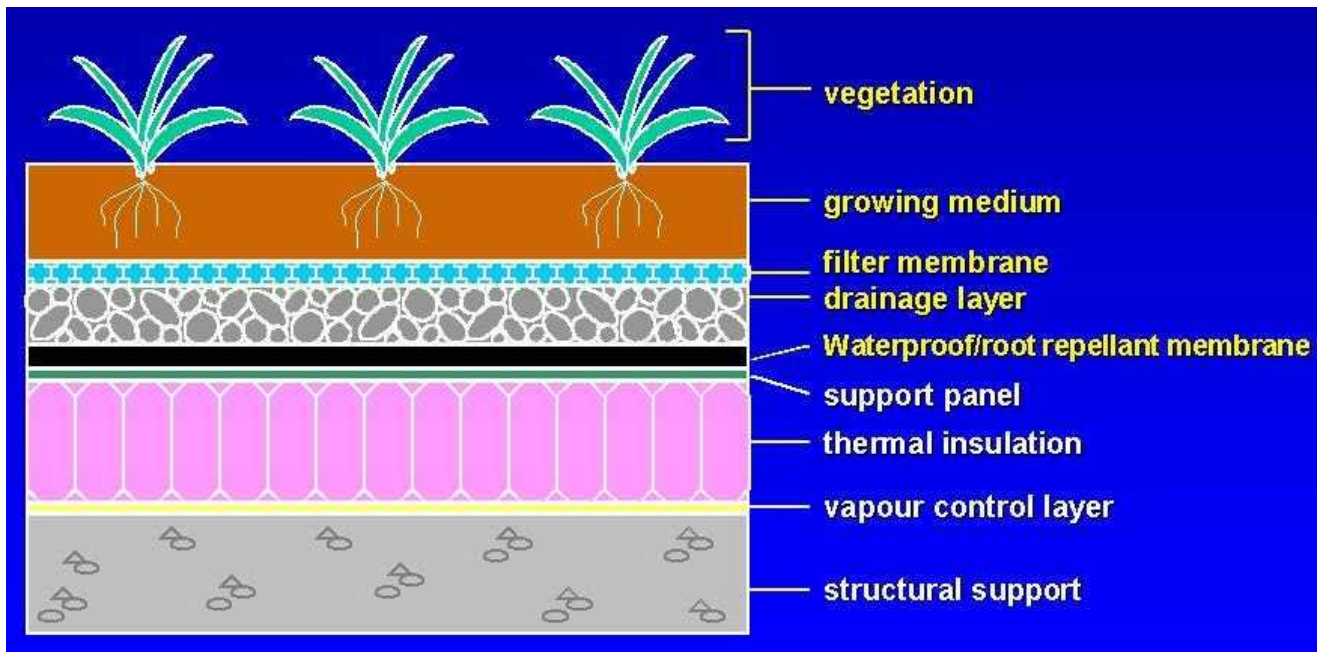

A green roof is represented by the BAHM2023 green roof element.

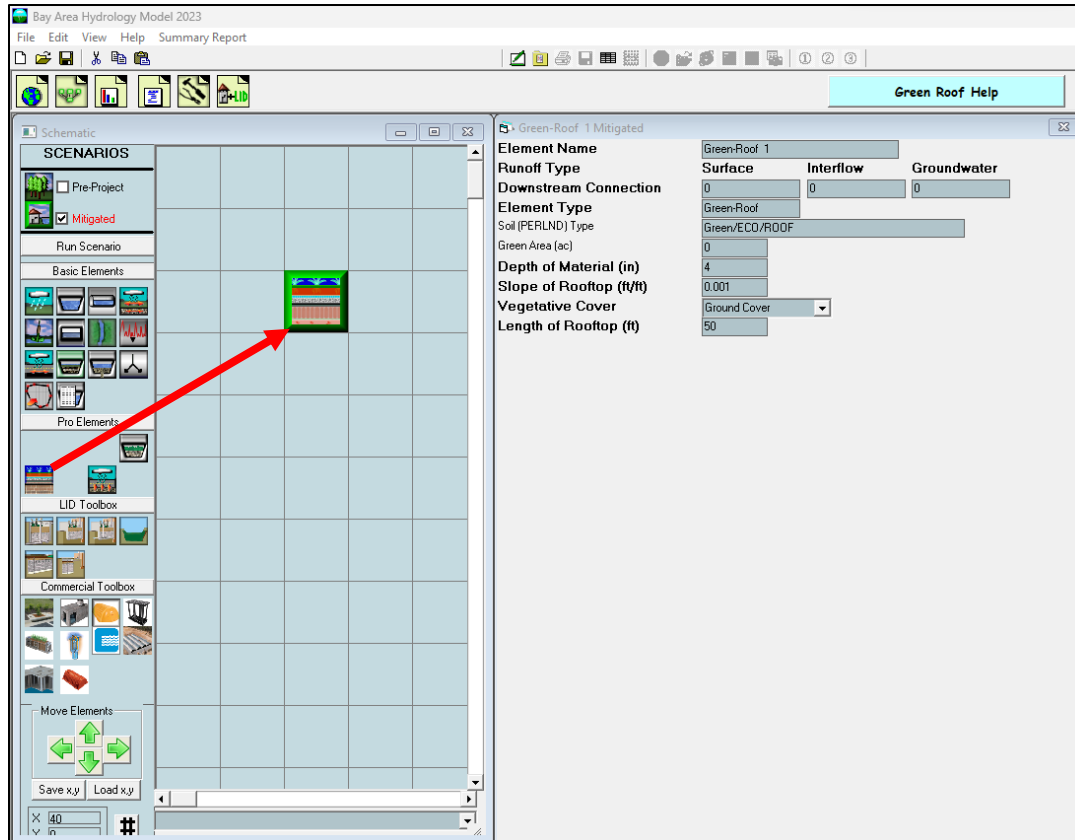

The dimensions and parameters to adjust to represent a green roof are:

Green Area (ac): Size of the green roof.

Depth of Material (in): Growing media/soil depth.

Slope of Rooftop (ft/ft): Roof surface slope.

Vegetative Cover: Type of vegetation on green roof (choices are: ground cover, shrubs, or trees).

Length of rooftop (ft): Length of the longest runoff path to reach a roof drain.

Default input values are automatically included with the element. They should be changed to reflect actual roof conditions.

The green roof surface area automatically receives rainfall and produces evapotranspiration. Due to this model input, the green roof surface area should be excluded from the basin element's total surface area.

If the green roof is connected to a downstream element or is selected as a point of compliance the user should make sure that the groundwater runoff is included. Unlike the other drainage area elements (basin element, etc.), the green roof groundwater always contributes to the total runoff. The green roof groundwater has nowhere else to go.

Learn more about the Green Roof element here:
www.clearcreeksolutions.info/bahm-course-home

RAINWATER HARVESTING

Rainwater harvesting involves water collection, storage, and reuse for residential outdoor use. The LID credit is pretty simple: the drainage area for which there is 100% capture does not have to be included in the BAHM2023 Mitigated land use scenario.



ADDITIONAL INFORMATION

The following pages contain additional information about these features:

- Outlet Structure Configurations
- Infiltration
- Auto Pond, Auto Vault, Auto Tank
- Stage-Storage-Discharge Table
- Point of Compliance
- Connecting Elements

OUTLET STRUCTURE CONFIGURATIONS

The trapezoidal pond, vault, tank, irregular pond, gravel trench bed, and sand filter all use a riser for the outlet structure to control discharge from the facility.

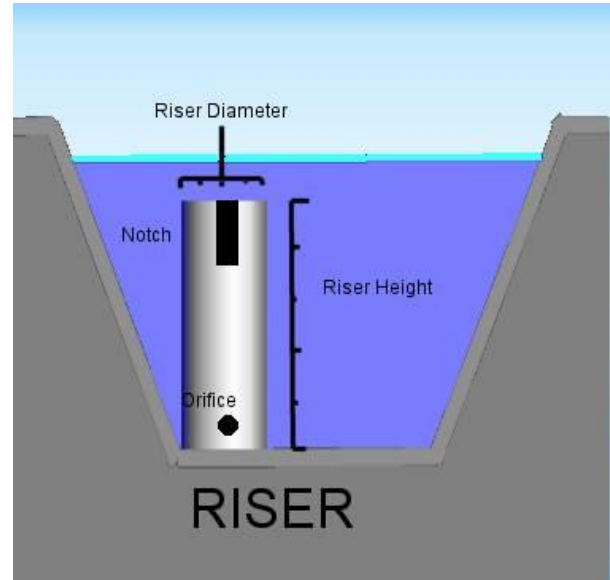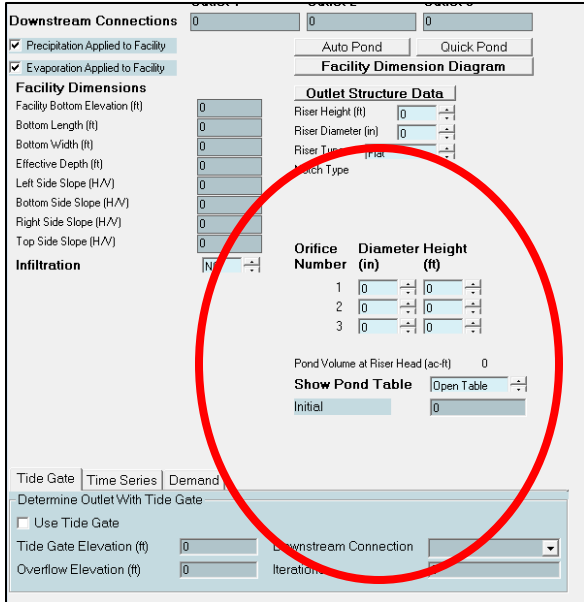

The riser is a vertical pipe with a height above pond bottom (typically one foot less than the effective depth). The user specifies the riser height and diameter.

The riser can have up to three round orifices. The bottom orifice is usually located at the bottom of the pond and/or above any dead storage in the facility. The user can set the diameter and height of each orifice.

Riser and Weir Representation.

The riser structure is a versatile structure that can be used to represent a weir, orifice, or culvert. A standard riser structure is intended to represent a circular standpipe. The standpipe diameter is user selected and can be any size. The Auto Size feature for all elements selects a default diameter for the riser but this can be adjusted after sizing is complete. The user is allowed to select up to three orifices that can be placed at any height inside the riser. The user can also select a notch in the riser. There are three options for the notch, rectangular, v-notch or Sutro.


Riser Weir

The top of a riser uses the weir equation to compute flow into the riser until the depth over the riser is greater than $\frac{1}{2}$ the diameter. As an example, if the riser is a 24-inch diameter riser then it will use the weir equation to compute flow until the water is more than 1 foot above the top of riser. In this way a riser can represent a transverse weir of any size. The key issue is to make sure that the circumference of the riser is equal to the length of the transverse weir.

Notched Riser Weir

A rectangular notch in a riser structure uses the transverse weir equation to compute the flow until the depth over the bottom of the notch is greater than ½ the notch height where it transitions to the orifice equation. In order to represent the weir correctly it is important to make sure that the diameter of the riser is greater than the weir length. For example, to model a 2-foot transverse weir the riser diameter needs to be at least 24 inches. Weir height is the actual height of the weir as measured down from the top of riser.

The user specifies the riser type as either flat or notched. The weir notch can be either rectangular, V-notch, or a Sutro weir. The shape of each type of weir is shown below.

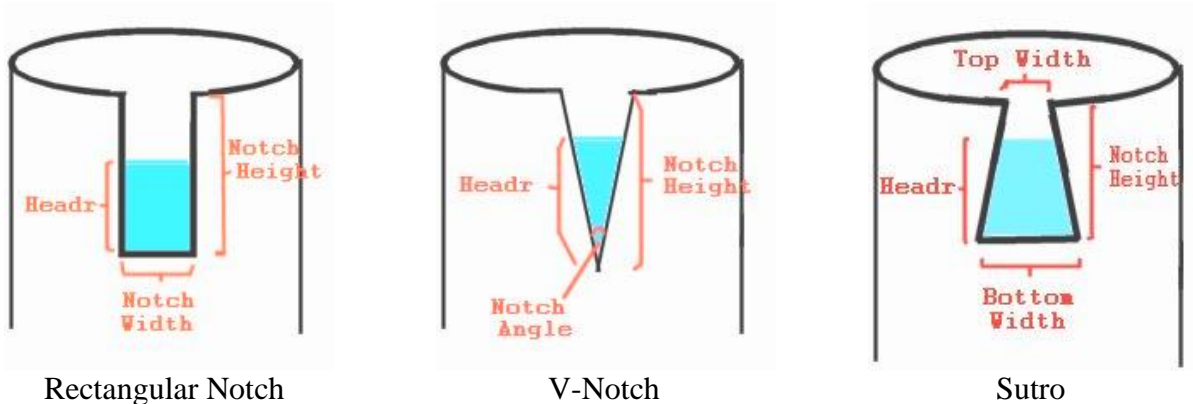

By selecting the appropriate notch type the user is then given the option to enter the appropriate notch type dimensions.

Riser and orifice equations used in BAHM2023 are provided below.

Headr = the water height over the notch/orifice bottom.

q = discharge

Riser Head Discharge:

$$\text{Head} = \text{water level above riser}$$

$$q = 9.739 * \text{Riser Diameter} * \text{Head}^{1.5}$$

Orifice Equation:

$$q = 3.782 * (\text{Orifice Diameter})^2 * \text{SQRT}(\text{Headr})$$

Rectangular Notch:

$$b = \text{NotchWidth} * (1 - 0.2 * \text{Headr})$$

where $b \geq 0.8$

$$q = 3.33 * b * \text{Headr}^{1.5}$$

Sutro:

$$\text{Wh} = \text{Top Width} + \{ (\text{Bottom Width} - \text{Top Width}) / \text{Notch Height} \} * \text{Headr}$$

Wd = Bottom Width - Wh (the difference between the bottom and top widths)

Q1 = (rectangular notch q where Notch Width = Wh)

Q2 = (rectangular notch q where Notch Width = Wd)

$$q = Q1 + Q2 / 2$$

V-Notch:

Notch Bottom = height from bottom of riser to bottom of notch

Theta = Notch Angle

$$a = 2.664261 - 0.0018641 * \text{Theta} + 0.00005761 * \text{Theta}^2$$

$$b = -0.48875 + 0.003843 * \text{Theta} - 0.000092124 * \text{Theta}^2$$


$$c = 0.3392 - 0.0024318 * \text{Theta} + 0.00004715 * \text{Theta}^2$$

$$\text{YoverH} = \text{Headr} / (\text{NotchBottom} + \text{Headr})$$

$$\text{Coef} = a + b * \text{Headr} + c * \text{Headr}^2$$

$$q = (\text{Coef} * \text{Tan}(\text{Theta} / 2)) * (\text{Headr}^{(5 / 2)})$$

These equations are provided from the Washington State Department of Ecology's 2005 *Stormwater Management Manual for Western Washington*. The outlet designs are shown below. They have been reproduced from Volume III of the *Stormwater Management Manual for Western Washington* which has more information on the subject.

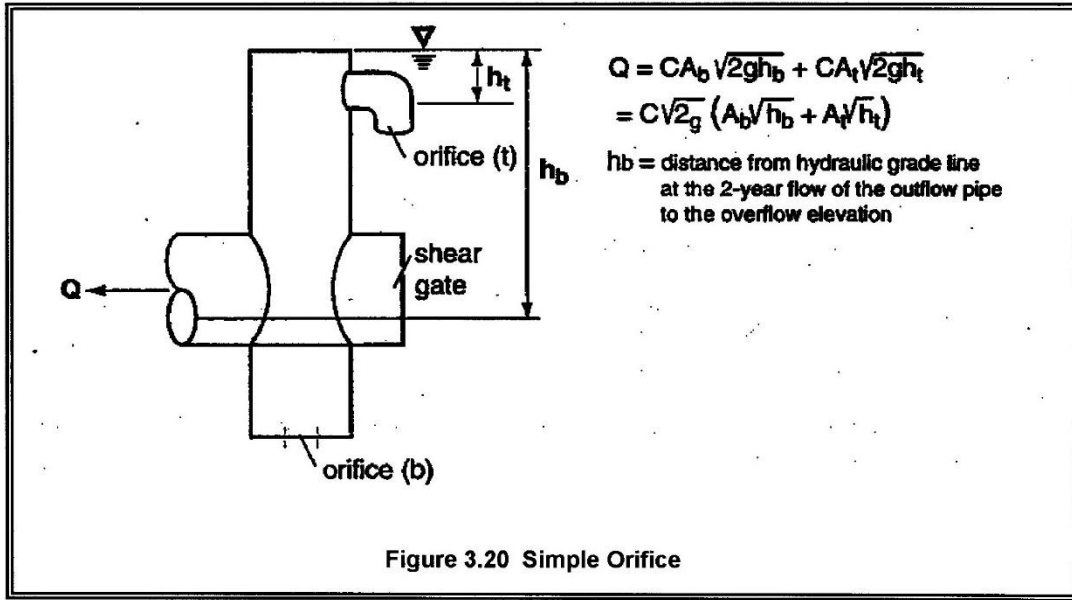

The diameter of the orifice is calculated from the flow. The orifice equation is often useful when expressed as the orifice diameter in inches:

$$d = \sqrt{\frac{36.88Q}{\sqrt{h}}} \quad (\text{equation 5})$$

where d = orifice diameter (inches)
 Q = flow (cfs)
 h = hydraulic head (ft)

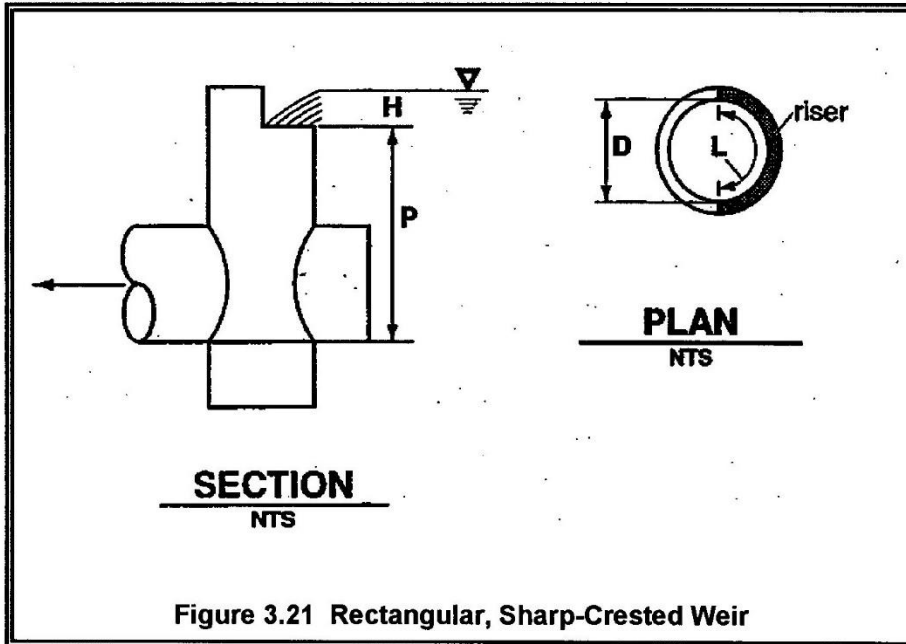


Figure 3.21 Rectangular, Sharp-Crested Weir

$$Q = C(L - 0.2H)H^{3/2} \quad (\text{equation 6})$$

where Q = flow (cfs)

$$C = 3.27 + 0.40 H/P \text{ (ft)}$$

H, P are as shown above

L = length (ft) of the portion of the riser circumference
as necessary not to exceed 50 percent of the

circumference

D = inside riser diameter (ft)

Note that this equation accounts for side contractions by subtracting $0.1H$ from L for each side of the notch weir.

The physical configuration of the outlet structure should include protection for the riser and orifices to prevent clogging of the outlet from debris or sediment. Various outlet configurations are shown below. They have been reproduced from Volume III of the *Stormwater Management Manual for Western Washington* which has more information on the subject.

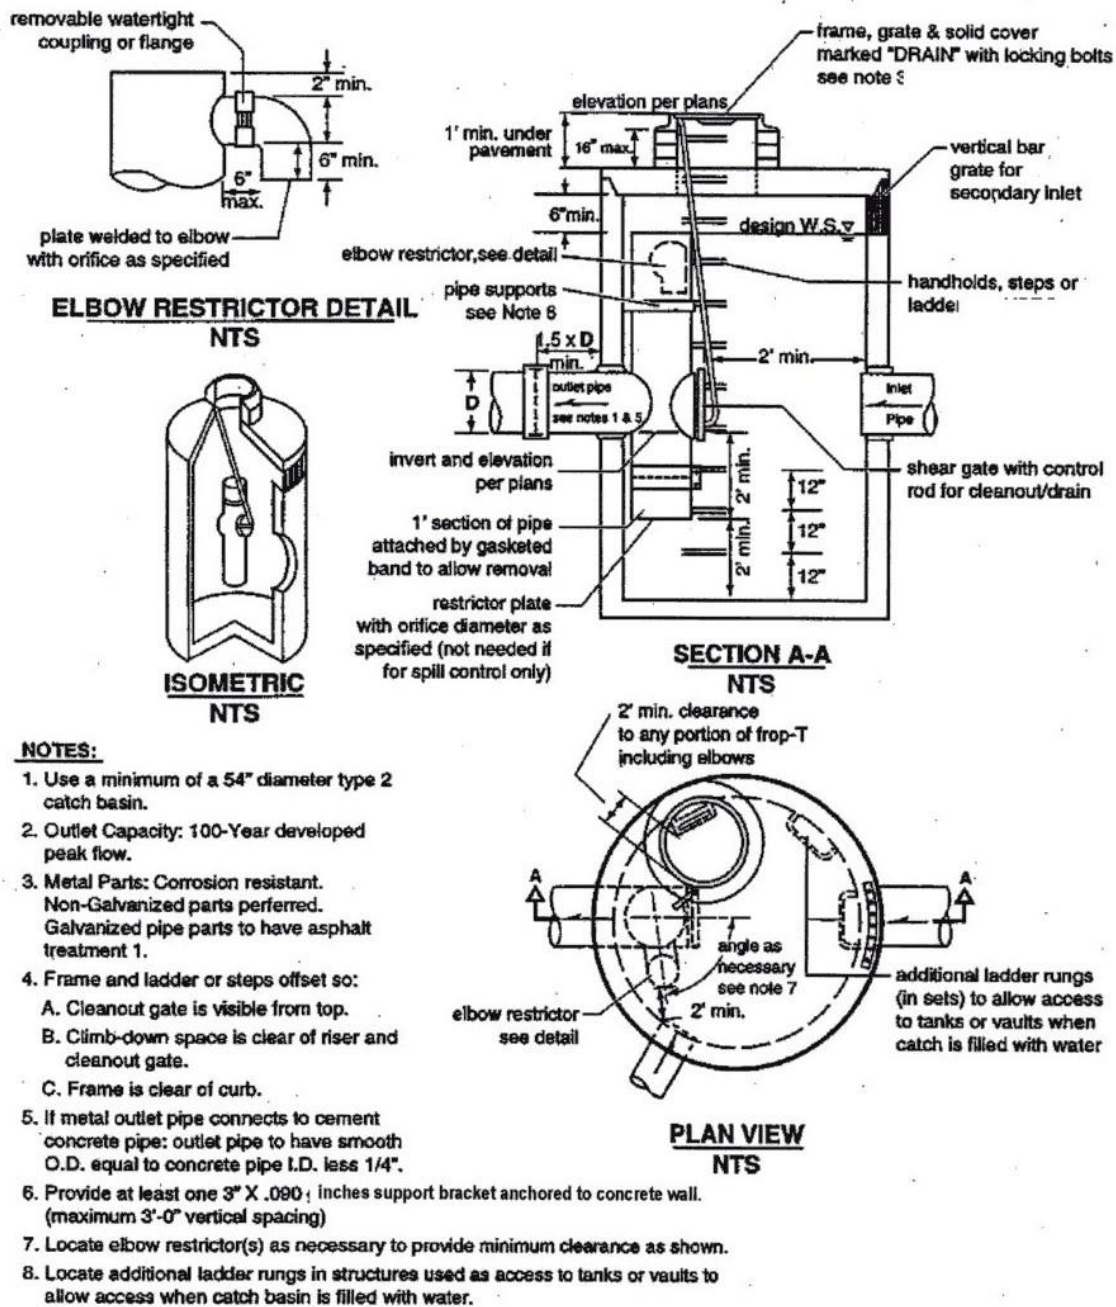


Figure 3.17 Flow Restrictor (TEE)

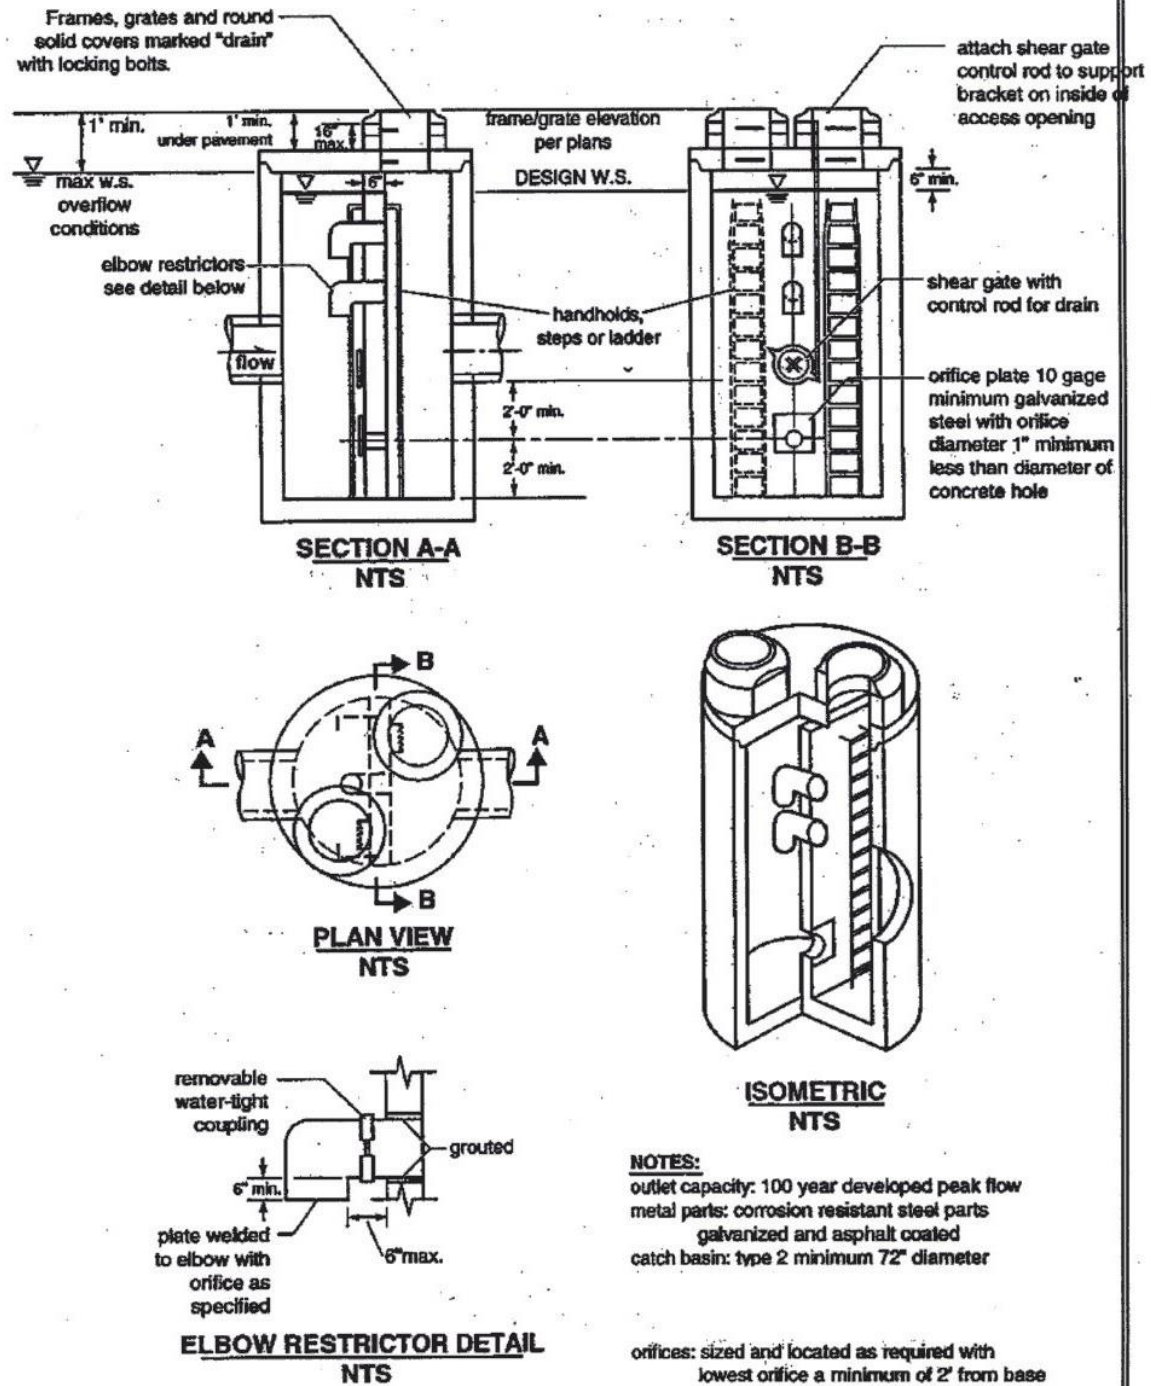


Figure 3.18 Flow Restrictor (Baffle)

Riser protection structures. Diagrams courtesy of Washington State Department of Ecology.

Included below is a conversion table relating the size of a rectangular opening for the riser with the size of a circular opening for the riser.

Surface Area of Rectangular Opening (sq-ft)	Diameter of Circular Opening (Feet)	Diameter of Circular Opening (Inches)
0.50	0.80	9.60
1.00	1.13	13.56
1.50	1.38	16.56
2.00	1.60	19.15
2.50	1.79	21.42
3.00	1.96	23.46
3.50	2.11	25.32
4.00	2.26	27.06
4.50	2.40	28.74
5.00	2.53	30.30
6.00	2.77	33.18
7.00	2.99	35.82
7.50	3.09	37.08
8.00	3.19	38.30
9.00	3.39	40.62
10.00	3.57	42.84
10.50	3.66	43.88
12.00	3.91	46.92
12.50	3.99	47.88
13.50	4.15	49.74
14.00	4.22	50.68
15.00	4.37	52.44
16.00	4.51	54.16
17.50	4.72	56.64
18.00	4.79	57.43
20.00	5.05	60.55
22.50	5.35	64.24

INFILTRATION

Infiltration of stormwater runoff is a recommended solution if certain conditions are met. These conditions include: a soils report, testing, groundwater protection, pre-treatment, and appropriate construction techniques.

NOTE: See Appendix D or consult with the local municipal permitting agency for additional considerations regarding infiltration and determination of the appropriate infiltration reduction factor.

The user clicks on the Infiltration option arrow to change infiltration from NO to YES. This activates the infiltration input options: measured infiltration rate, infiltration reduction factor, and whether or not to allow infiltration through the wetted side slopes/walls.

The screenshot shows the 'Trapezoidal Pond 1 Mitigated' configuration window. The 'Infiltration' section is circled in red. It contains the following fields:

- Infiltration:**
 - Measured Infiltration Rate (in/hr): 0
 - Reduction Factor (infiltration factor): 1
 - Use Wetted Surface Area (sidewalls): NO
 - Total Volume Infiltrated (ac-ft): 0
 - Total Volume Through Riser (ac-ft): 0
 - Total Volume Through Facility (ac-ft): 0.00
 - Percent Infiltrated: 0
- Facility Dimensions:**
 - Facility Bottom Elevation (ft): 0
 - Bottom Length (ft): 200
 - Bottom Width (ft): 200
 - Effective Depth (ft): 4
 - Left Side Slope (H/V): 3
 - Bottom Side Slope (H/V): 3
 - Right Side Slope (H/V): 3
 - Top Side Slope (H/V): 3
- Outlet Structure Data:**
 - Riser Height (ft): 3
 - Riser Diameter (in): 24
 - Riser Type: Notched
 - Notch Type: Rectangular
 - Notch Height (ft): 1
 - Notch Width (ft): 2
- Orifice:**
 - Orifice Number: 1, 2, 3
 - Diameter (in): 3, 0, 0
 - Height (ft): 0, 0, 0
- Other Settings:**
 - Pond Volume at Riser Head (ac-ft): 3.034
 - Initial: 0
 - Target %: 100
 - Iterations: 0


The infiltration reduction factor is a multiplier for the measured infiltration rate and should be less than one. It is the same as the inverse of a safety factor. For example, a safety factor of 2 is equal to a reduction factor of 0.5.

Infiltration occurs only through the bottom of the facility if the wetted surface area option is turned off. Otherwise, the entire wetted surface area is used for infiltration.

After the model is run and flow is routed through the infiltration facility, the total volume infiltrated, total volume through the riser, total volume through the facility, and percent infiltrated are reported on the screen. If the percent infiltrated is 100%, then there is no surface discharge from the facility. The percent infiltrated can be less than 100% as long as the surface discharge does not exceed the flow duration criteria.

Infiltration facilities have the option to allow users to automatically size the facility to meet an infiltration target percentage. The user can set the target percentage for being filtered/infiltrated to 80% to meet the water quality treatment standard.

AUTO POND, AUTO VAULT, AUTO TANK

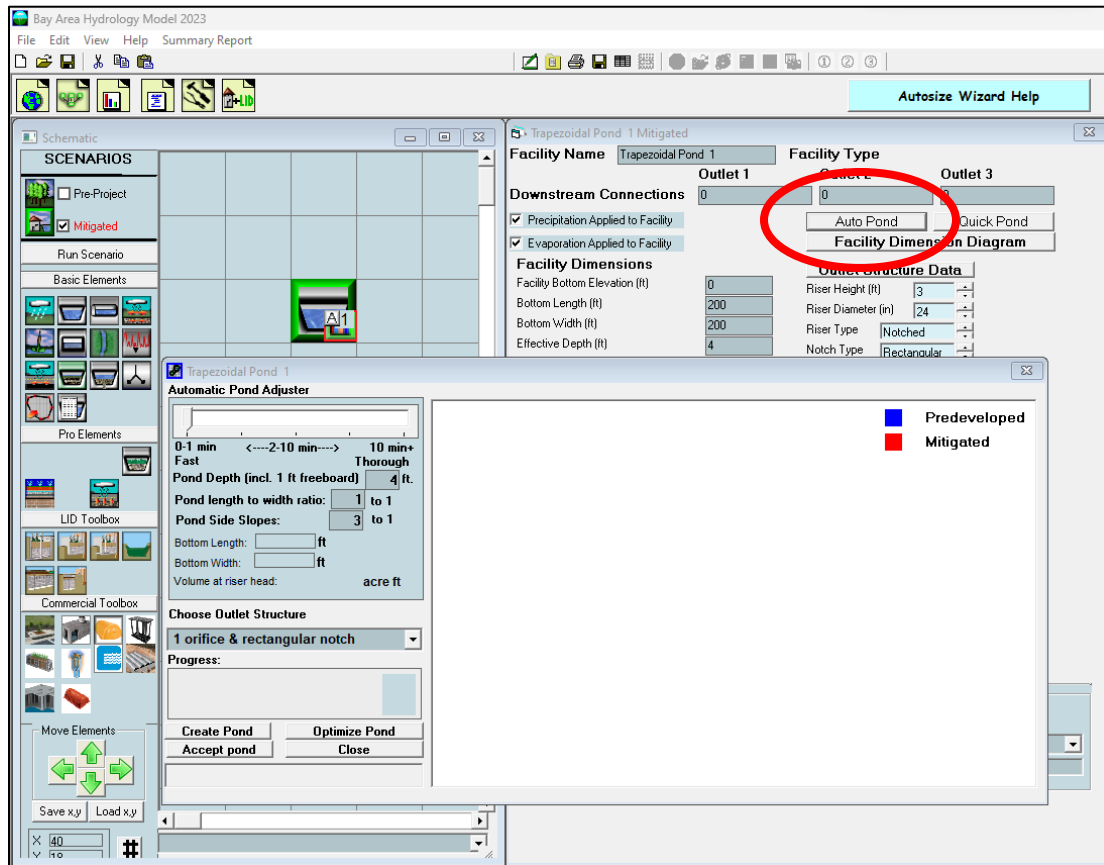

Auto Pond, Auto Vault, and Auto Tank all work the same. Each optimizing routine automatically creates a pond, vault, or tank size and designs the outlet structure to meet the flow duration criteria. The user can either create a pond, vault, or tank from scratch or optimize an existing design.

The following information applies to all three optimizing routines (Auto Pond, Auto Vault, and Auto Tank), but for the purposes of simplifying the following documentation the term “Auto Pond” applies equally to Auto Vault and Auto Tank.

Auto Pond requires that the Pre-project and Mitigated basins be defined prior to using Auto Pond. Clicking on the Auto Pond button brings up the Auto Pond window and the associated Auto Pond controls.

Auto Pond controls:

Automatic Pond Adjuster: The slider at the top of the Auto Pond window allows the user to decide how thoroughly the pond will be designed for efficiency. The lowest setting (0-1 min) at the left constructs an initial pond without checking the flow duration criteria. The second setting to the right creates and sizes a pond to pass the flow duration criteria;

however, the pond is not necessarily optimized. The higher settings increase the amount of optimization. The highest setting (farthest left) will size the most efficient (smallest) pond but will result in longer computational time.

Pond Depth: Pond depth is the total depth of the pond and should include at least one foot of freeboard (above the riser). The pond's original depth will be used when optimizing an existing pond; changing the value in the Pond Depth text box will override any previous set depth value. The default depth is 4 feet.

Pond Length to Width Ratio: This bottom length to width ratio will be maintained regardless of the pond size or orientation. The default ratio value is 1.0.

Pond Side Slopes: Auto Pond assumes that all of the pond's sides have the same side slope. The side slope is defined as the horizontal distance divided by the vertical. A typical side slope is 3 (3 feet horizontal to every 1 foot vertical). The default side slope value is 3.

Choose Outlet Structure: The user has the choice of either 1 orifice and rectangular notch or 3 orifices. If the user wants to select another outlet structure option, then the pond must be manually sized.

Create Pond: This button creates a pond when the user does not input any pond dimensions or outlet structure information. Any previously input pond information will be deleted.

Optimize Pond: This button optimizes an existing pond. It cannot be used if the user has not already created a pond.

Accept Pond: This button will stop the Auto Pond routine at the last pond size and discharge characteristics that produce a pond that passes the flow duration criteria. Auto Pond will not stop immediately if the flow duration criteria have not yet been met.

The bottom length and width and volume at riser head will be computed by Auto Pond; they cannot be input by the user.

AutoVault operates the same way as Auto Pond.

There are some situations where Auto Pond will not work. These situations occur when complex routing conditions upstream of the pond make it difficult or impossible for Auto Pond to determine which land use will be contributing runoff to the pond. For these situations the pond will have to be manually sized. Go to page 46 to find information on how to manually size a pond or other HM facility.

NOTE: *If Auto Pond selects a bottom orifice diameter smaller than the smallest diameter allowed by the local municipal permitting agency then the user has the option of specifying a minimum allowable bottom orifice diameter even if this size*

diameter is too large to meet flow duration criteria for this element. Additional mitigating BMPs may be required to meet local hydromodification control requirements. Please see Appendix D or consult with local municipal permitting agency for more details. For manual sizing information see page 46.

Learn more about Auto-Sizing Features here:
www.clearcreeksolutions.info/bahm-course-home

STAGE-STORAGE-DISCHARGE TABLE

Stage (ft)	Area (acres)	Storage (acre-ft)	Dschrge (cfs)	Infiltr (cfs)
0.000000	0.918274	0.000000	0.000000	0.000000
0.044444	0.920724	0.040867	0.051488	0.000000
0.088889	0.923178	0.081842	0.072816	0.000000
0.133333	0.925635	0.122927	0.089181	0.000000
0.177778	0.928095	0.164121	0.102977	0.000000
0.222222	0.930558	0.205424	0.115132	0.000000
0.266667	0.933025	0.246837	0.126120	0.000000
0.311111	0.935495	0.288360	0.136226	0.000000
0.355556	0.937968	0.329992	0.145631	0.000000
0.400000	0.940444	0.371735	0.154465	0.000000
0.444444	0.942924	0.413588	0.162821	0.000000
0.488889	0.945407	0.455550	0.170768	0.000000
0.533333	0.947893	0.497624	0.178361	0.000000
0.577778	0.950383	0.539808	0.185644	0.000000
0.622222	0.952876	0.582102	0.192652	0.000000
0.666667	0.955372	0.624508	0.199414	0.000000
0.711111	0.957871	0.667024	0.205954	0.000000
0.755556	0.960374	0.709652	0.212292	0.000000
0.800000	0.962880	0.752391	0.218447	0.000000
0.844444	0.965389	0.795241	0.224433	0.000000
0.888889	0.967901	0.838203	0.230263	0.000000
0.933333	0.970417	0.881277	0.235950	0.000000
0.977778	0.972936	0.924463	0.241502	0.000000
1.022222	0.975458	0.967760	0.246930	0.000000
1.066667	0.977983	1.011170	0.252241	0.000000
1.111111	0.980512	1.054692	0.257442	0.000000
1.155556	0.983044	1.098327	0.262541	0.000000
1.200000	0.985579	1.142074	0.267542	0.000000
1.244444	0.988118	1.185934	0.272451	0.000000
1.288889	0.990660	1.229907	0.277274	0.000000
1.333333	0.993205	1.273993	0.282014	0.000000
1.377778	0.995753	1.318192	0.286676	0.000000
1.422222	0.998305	1.362504	0.291263	0.000000
1.466667	1.000860	1.406930	0.295779	0.000000
1.511111	1.003418	1.451470	0.300227	0.000000
1.555556	1.005979	1.496123	0.304610	0.000000


The stage-storage-discharge table hydraulically represents any facility that requires stormwater routing. The table is automatically generated by BAHM2023 when the user inputs storage facility dimensions and outlet structure information. BAHM2023 generates 91 lines of stage, surface area, storage, surface discharge, and infiltration values starting at a stage value of zero (facility bottom height) and increasing in equal increments to the maximum stage value (facility effective depth).

When the user or BAHM2023 changes a facility dimension (for example, bottom length) or an orifice diameter or height, the model immediately recalculates the stage-storage-discharge table.

The user can input to BAHM2023 a stage-storage-discharge table created outside of BAHM2023. To use a stage-storage-discharge table created out of BAHM2023, the SSD Table element is required (see page 68). See the SSD Table element description on page 68 for more information on how to load such a table to BAHM2023 program.

POINT OF COMPLIANCE

BAHM2023 allows for multiple points of compliance (maximum of 59) in a single project. A point of compliance is defined as the location at which the Pre-project and Mitigated flows will be analyzed for compliance with the flow control standard.

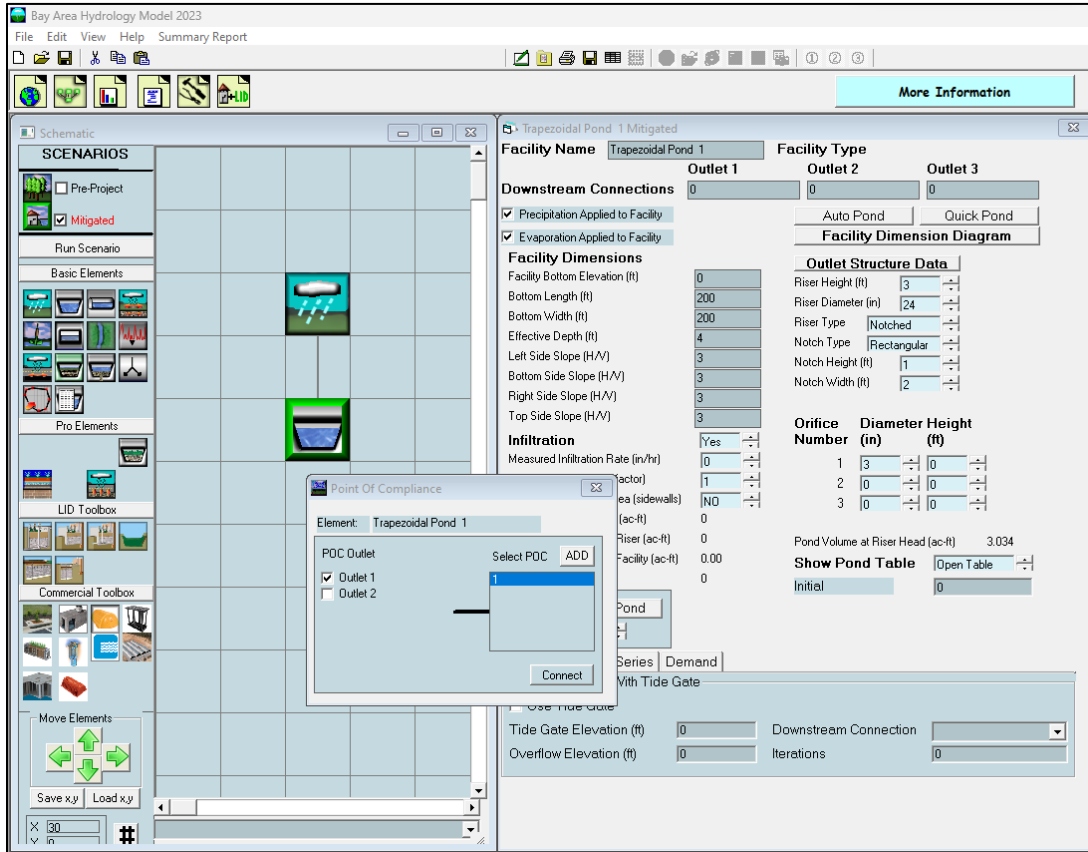


The point of compliance is selected by right clicking on the element at which the compliance analysis will be made. In the example above, the point of compliance analysis will be conducted at the outlet of the trapezoidal pond.

Once the point of compliance has been selected the element is modified on the Schematic screen to include a small box with the letter “A” (for Analysis) in the lower right corner. This identifies the outlet from this element as a point of compliance.


The number 1 next to the letter “A” is the number of the POC (POC 1).



CONNECTING ELEMENTS

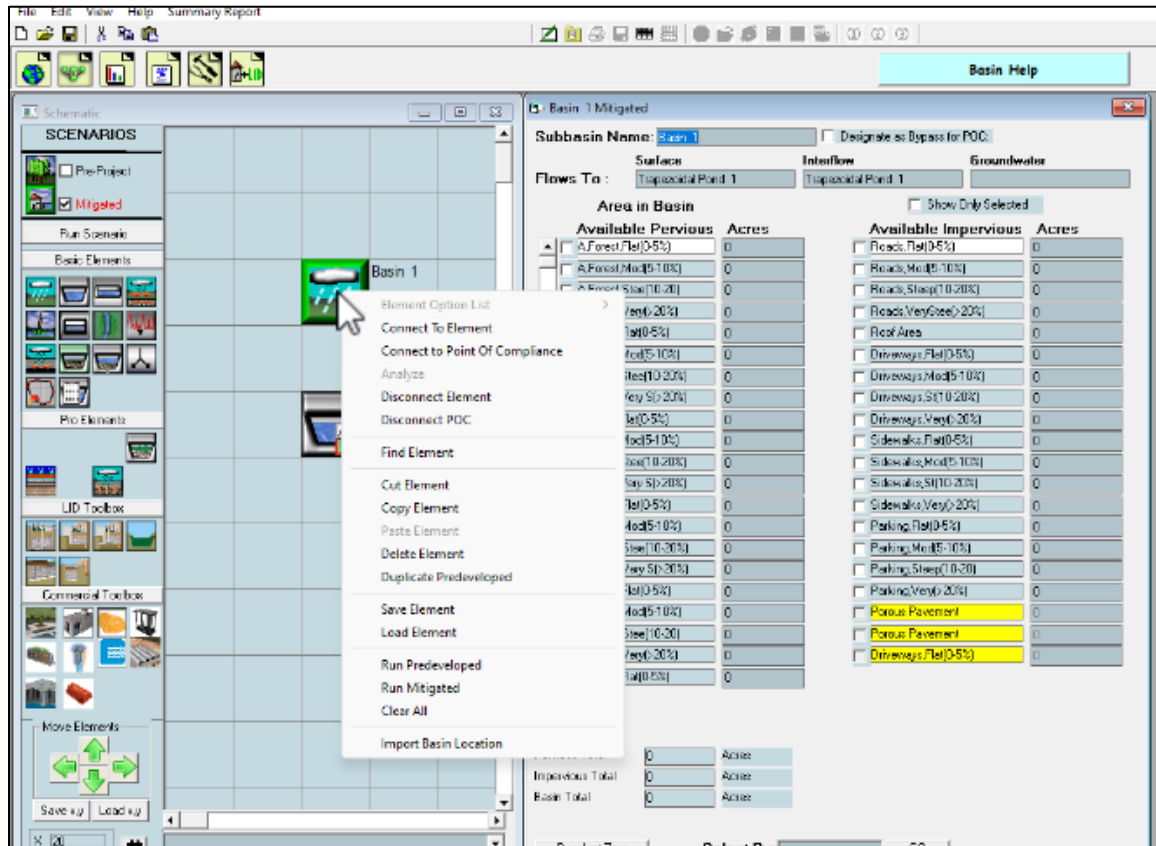


Elements are connected by right clicking on the upstream element (in this example Basin 1) and selecting and then left clicking on the Connect To Element option. By doing so, BAHM2023 extends a line from the upstream element to wherever the user wants to connect that element.

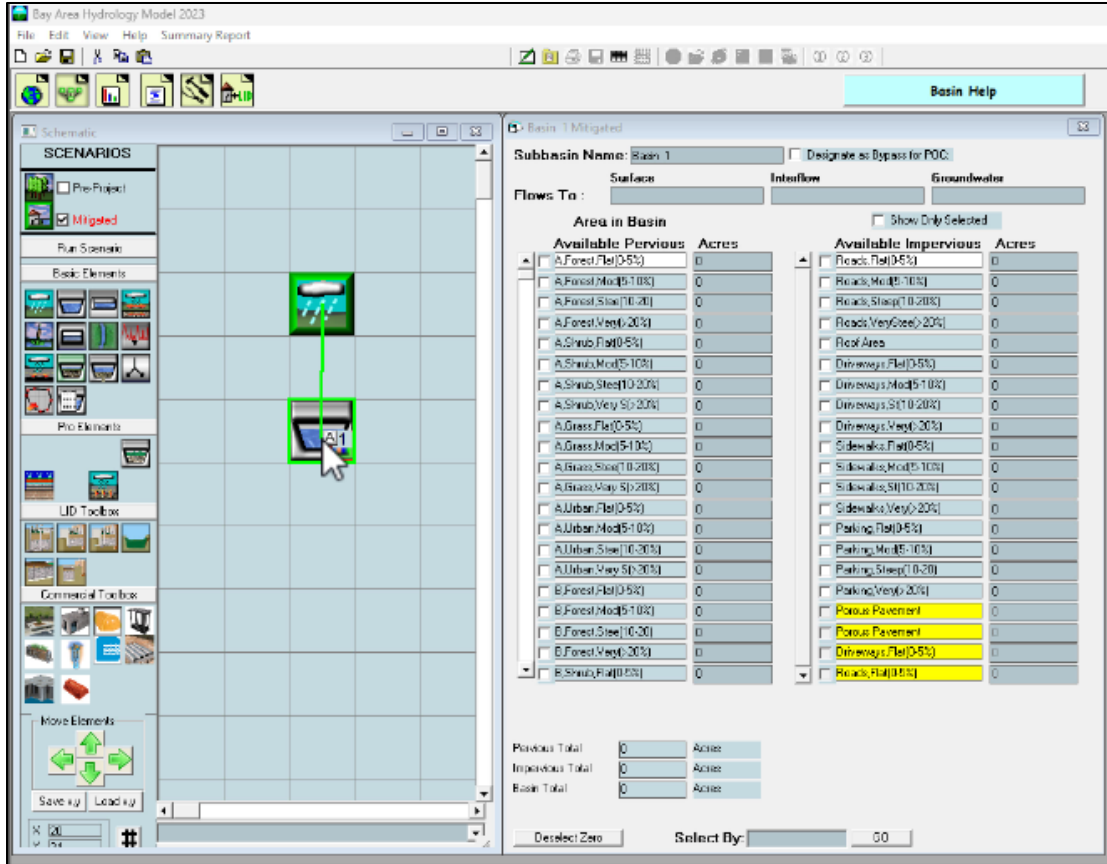


The user extends the connection line to the downstream element (in this example, a pond) and left clicks on the destination element. This action brings up the From Basin to Conveyance box that allows the user to specify which runoff components to route to the downstream element.

Stormwater runoff is defined as surface flow + interflow. Both boxes should be checked. Groundwater should not be checked for the standard land development mitigation analysis. Groundwater should only be checked when there is observed and documented base flow occurring from the upstream basin.

After the appropriate boxes have been checked click the OK button.

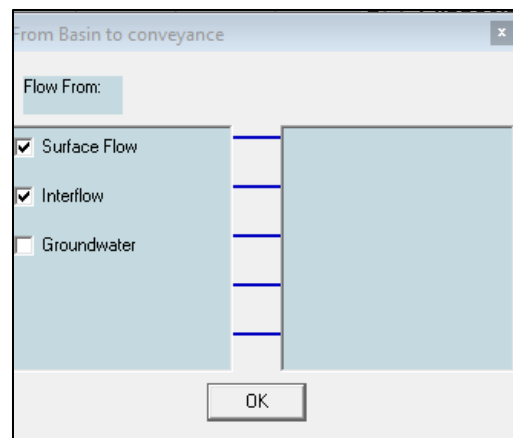


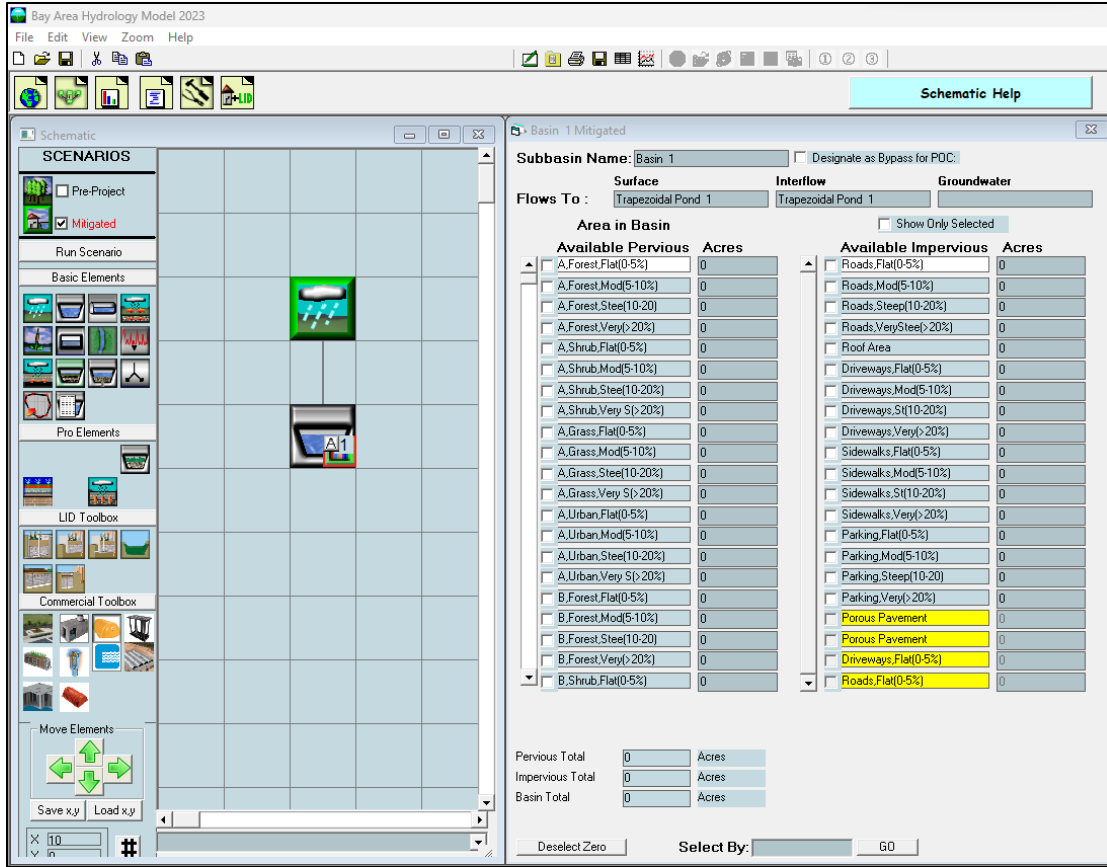


The final screen will look like the above screen. The basin information screen on the right will show that Basin 1 surface and interflow flows to Trapezoidal Pond 1 (groundwater is not connected).

This page has been intentionally left blank.

ANALYSIS SCREEN

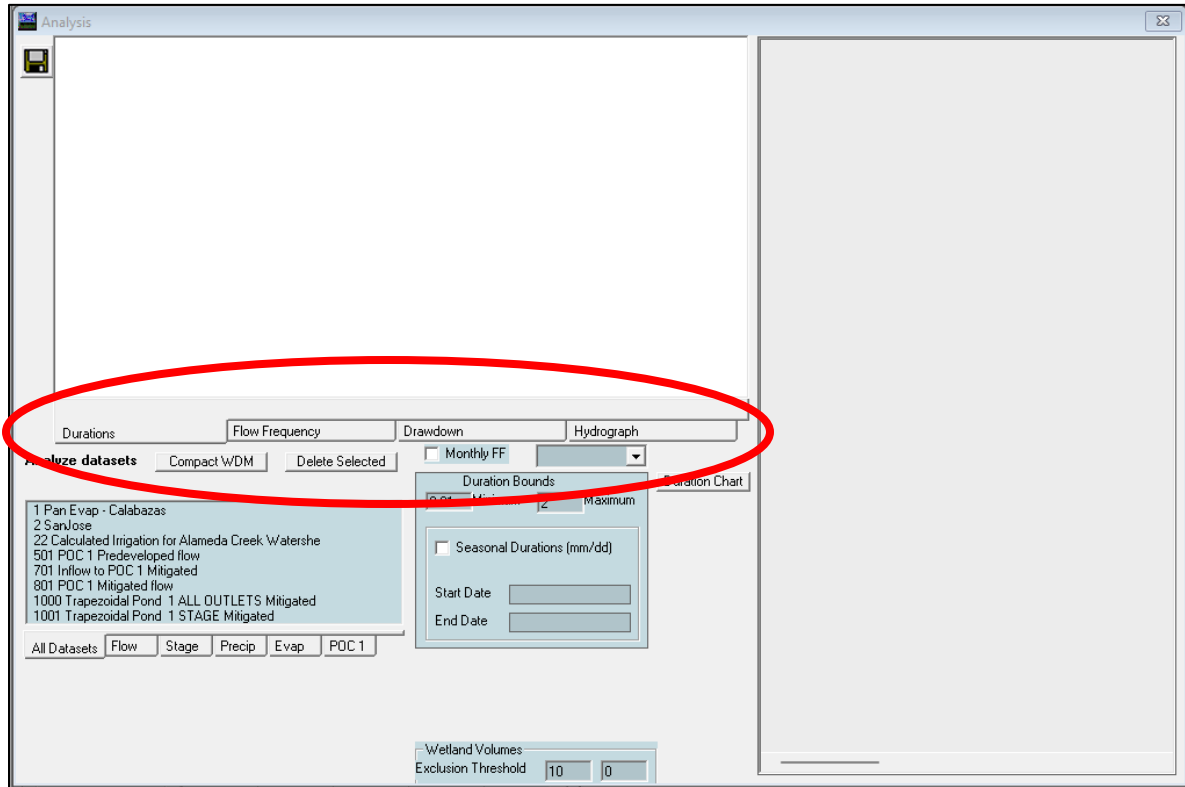


The Analysis tool bar button (third from the left) brings up the Analysis screen where the user can look at the results. The Analysis screen allows the user to analyze and compare flow durations, flow frequency, drawdown times, and hydrographs.

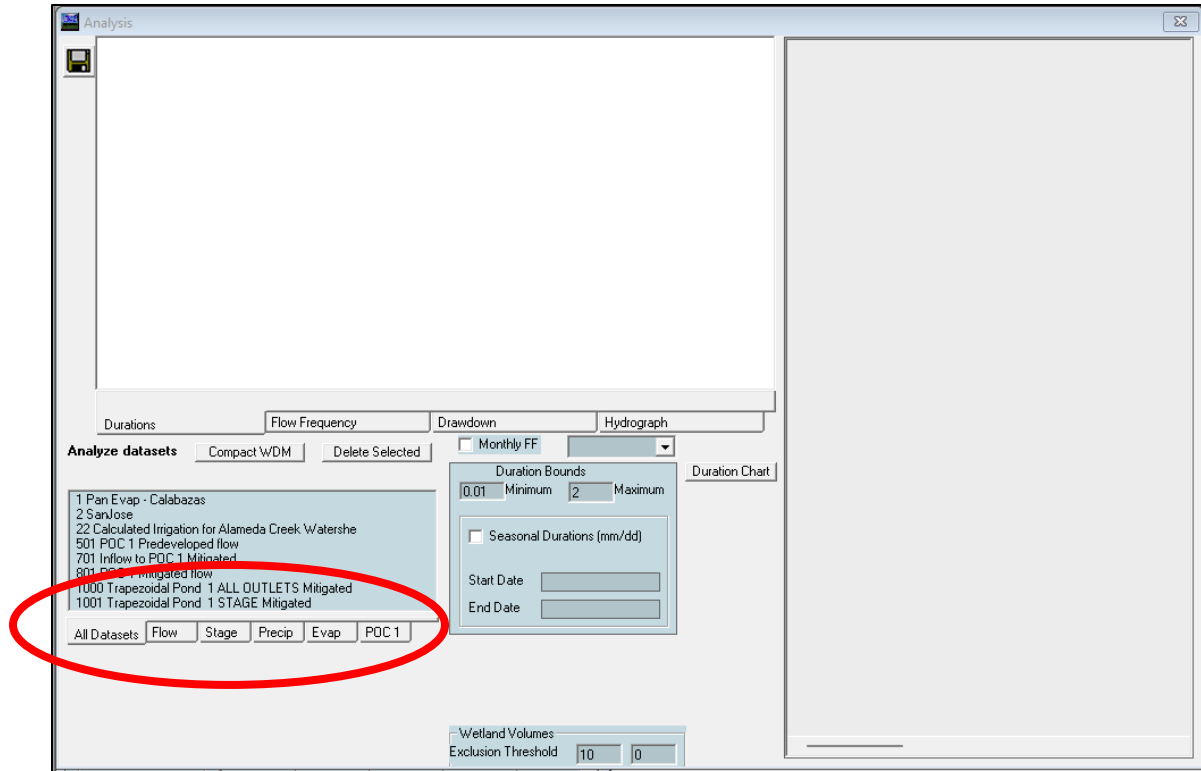

The user can analyze all time series datasets or just flow, stage, precipitation, evaporation, or point of compliance (POC) flows by selecting the appropriate tab below the list of the different datasets available for analysis.

Learn more about the Analysis Screen here:
www.clearcreeksolutions.info/bahm-course-home

FLOW DURATION

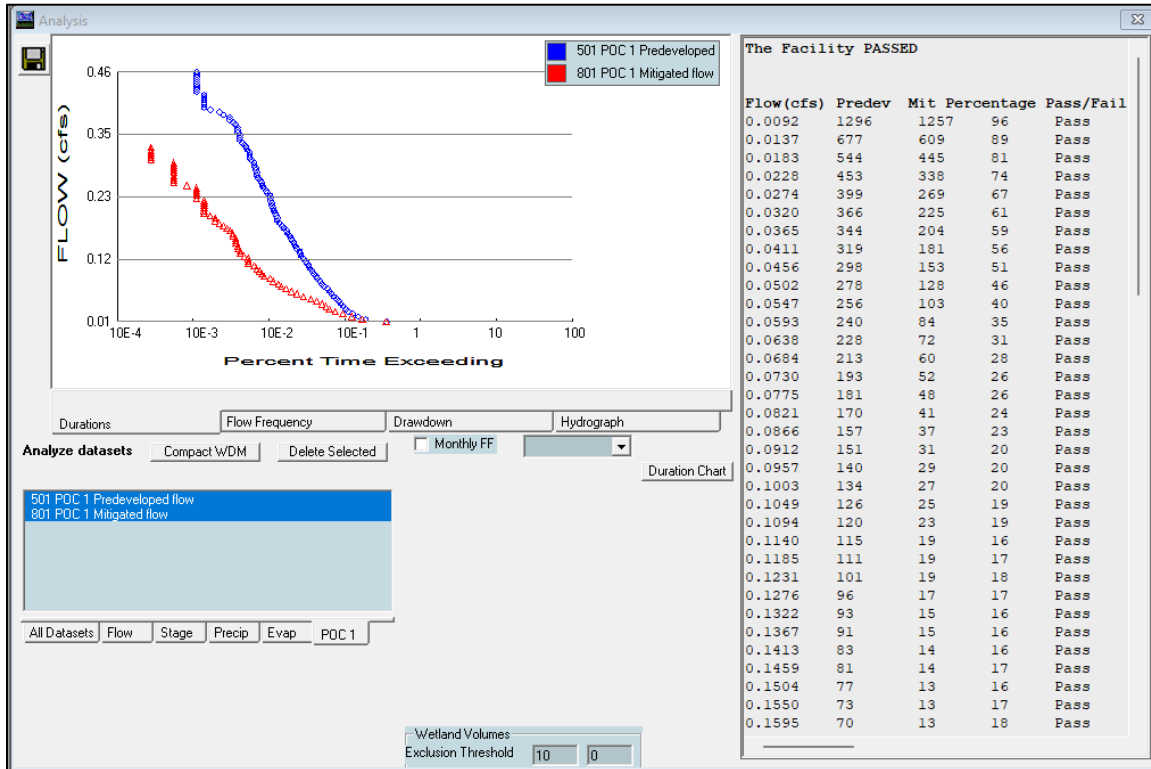


Flow duration at the point of compliance (POC 1) is the most common analysis. A plot of the flow duration values is shown on the left, the flow values on the right.

The flow duration flow range is from 10% of the 2-year flow frequency value to the 10-year value. As shown in the flow duration table to the right of the flow duration curves, this flow range is divided into approximately 100 levels (flow values). For each flow level/value, BAHM2023 counts the number of times that the flow at the Point of Compliance for the Pre-project scenario (Predev) exceeds that specific flow level/value. It does the same count for the Mitigated scenario flow (Dev). The total number of counts is the number of simulated hours in the multi-year simulation period that the flow exceeds that specific flow level/value.

The Percentage column is the ratio of the Dev count to the Predev count. This ratio must be less than or equal to 110.0 for flow levels/values between 10% of the 2-year flow value and the 10-year value (the upper limit)¹⁵. If the percentage value does not exceed this maximum ratio (110% for 10% of the 2-year value to the 10-year value) then the Pass/Fail column shows a Pass for that flow level. If they are exceeded, then a Fail is shown. One Fail and the facility fails the flow duration criteria. The facility overall Pass/Fail is listed at the top of the flow duration table.

¹⁵ The goodness of fit criteria in the Municipal Regional Permit is as follows: the post-project flow duration curve shall not deviate above the pre-project flow duration curve by more than 10 percent over more than 10 percent of the length of the curve corresponding to the range of flows to control.

FLOW FREQUENCY

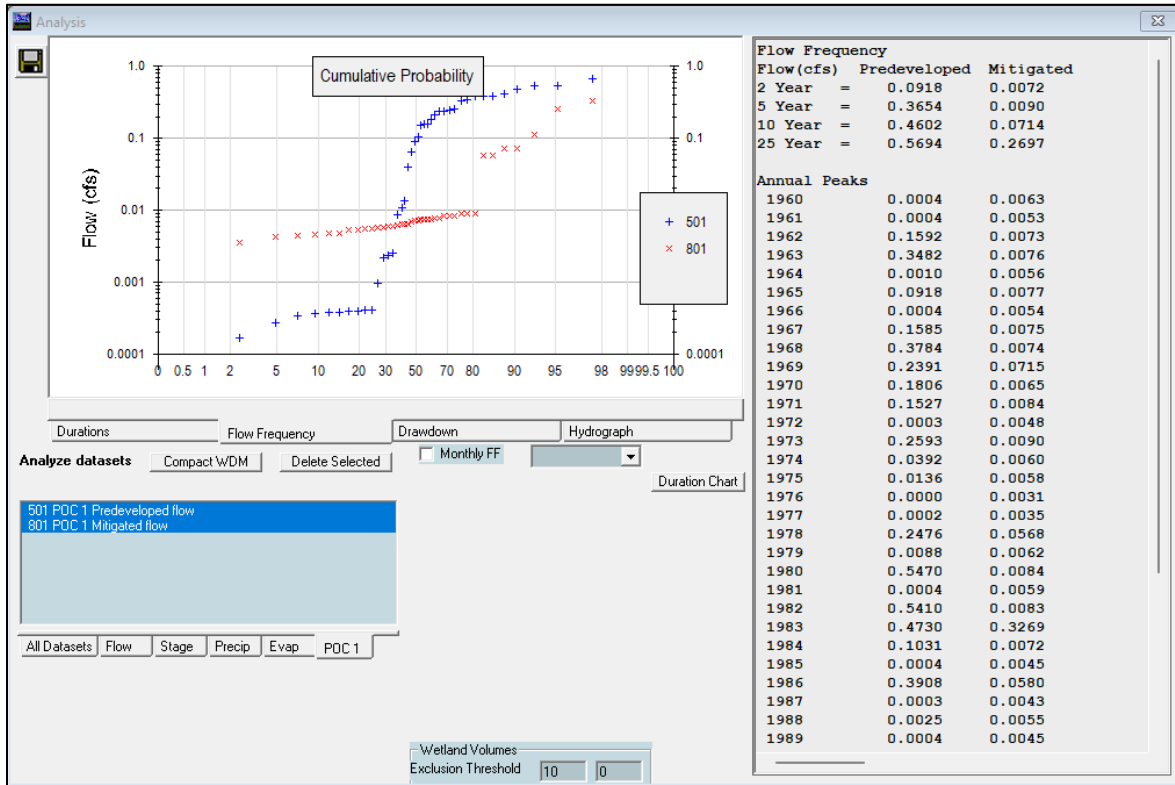

Flow frequency plots are shown on the left and the 2-, 5-, 10-, and 25-year frequency values are on the right. Flow frequency calculations are based on selecting annual peak flow values and ranking them by their Weibull Plotting Position.

The Weibull Plotting Position formula is:

$$P = (m-a)/(N-a-b+1)$$

where P = probability
 m = rank
 N = number of years
 a = constant
 b = constant

The two constants (a and b) are used to adjust the probability of historical values to more accurately represent extreme events (for example, 100-year event) when the number of years (N) is not sufficient to produce the appropriate Weibull plotting position. For the purposes of the HM requirements, which focuses on the range of 10% of the 2-year to the 10-year, the constants can be assumed to equal zero. This reduces the Weibull equation to


$$P = m/(N+1)$$

Return period, Tr (years) = 1/P

The return period value, T_r , is used in BAHM2023 to determine the 2-year, 5-year, 10-year, and 25-year peak flow values. If necessary, the 2-year, 5-year, 10-year, and 25-year values are interpolated from the T_r values generated by Weibull.

Learn more about the Flow Frequency here:
www.clearcreeksolutions.info/bahm-course-home

DRAWDOWN

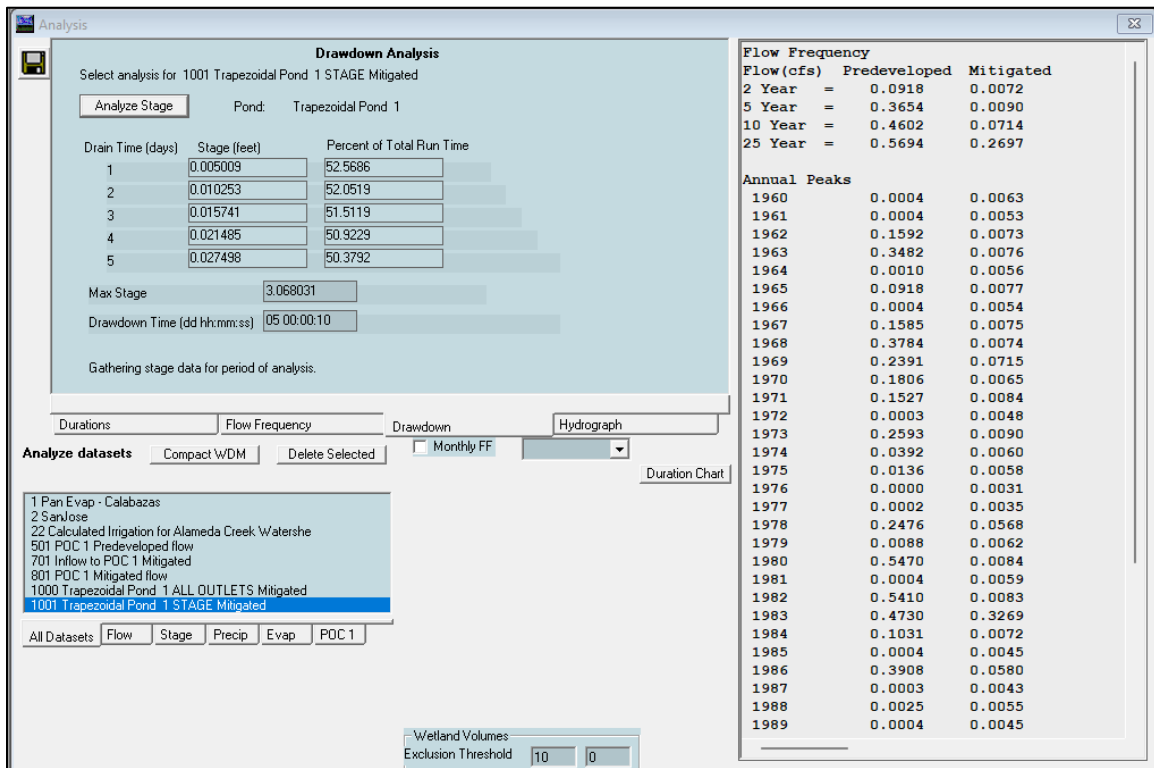

The drawdown screen is used to compute pond stages (water depths). These stages are summarized and reported in terms of drain/retention time (in days).

For this example, the maximum stage computed during the entire 35-50 year simulation period is 3.07 feet. This maximum stage has a drawdown time of 5 days.


Stages can have drain times in excess of 5 days. This can occur when a pond has a small bottom orifice. If this is not acceptable, then the user needs to change the pond outlet configuration, manually run the Mitigated scenario, and repeat the analyze stage computations. A situation may occur where it is not possible to have both an acceptable pond drawdown/retention time and meet the flow duration criteria.

NOTE: The flow duration criteria take precedence unless the user is instructed otherwise by the local municipal permitting agency.

Learn more about Drawdown here:

www.clearcreeksolutions.info/bahm-course-home

HYDROGRAPHS

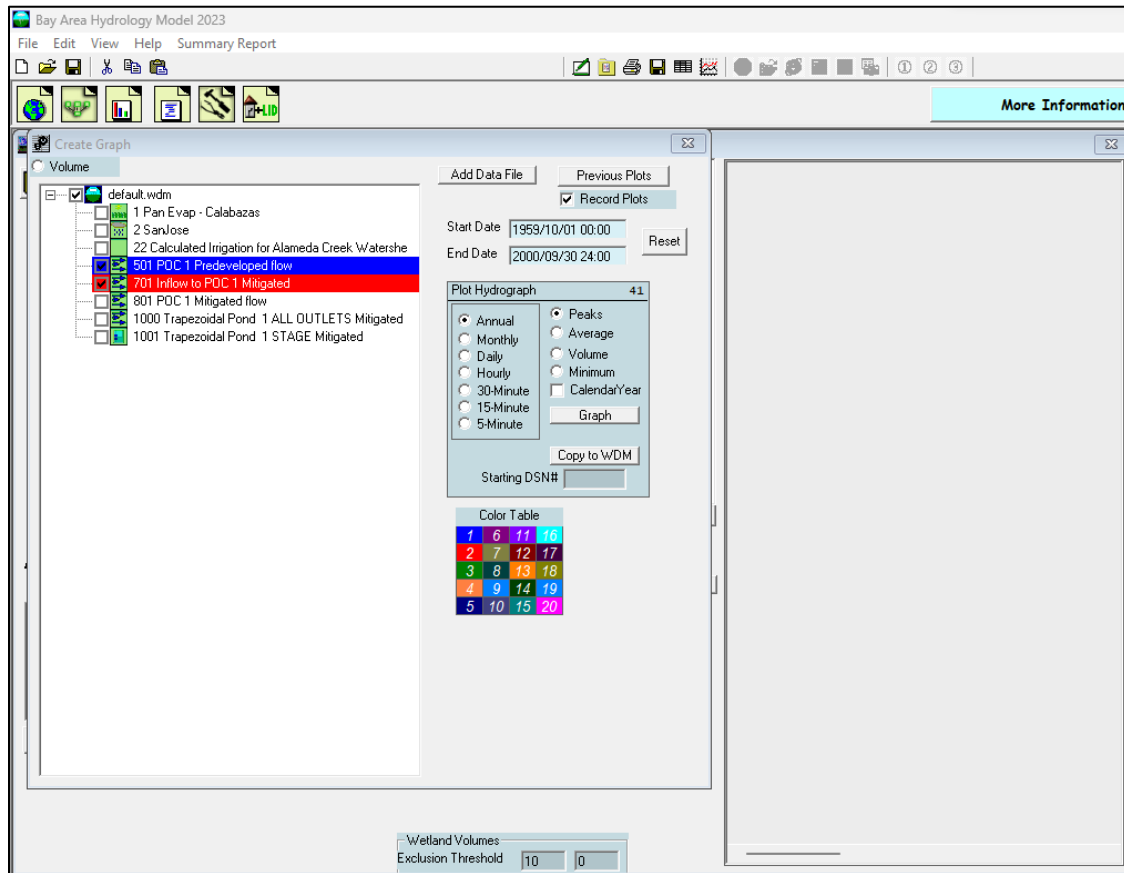

The user can graph/plot any or all time series data by selecting the Hydrograph tab. The Create Graph screen is shown, and the user can select the time series to plot, the time interval (yearly, monthly, daily, or hourly), and type of data (peaks, average, or volume).


The following numbering system is used for the flow time series:

500-599: Pre-project flow (Pre-project scenario)

700-799: Pre-mitigated flow (Mitigated scenario before the pond)

800-899: Mitigated flow (Mitigated scenario after the pond)


The selected time series are shown. To graph the selected time series the user clicks on the Graph button.

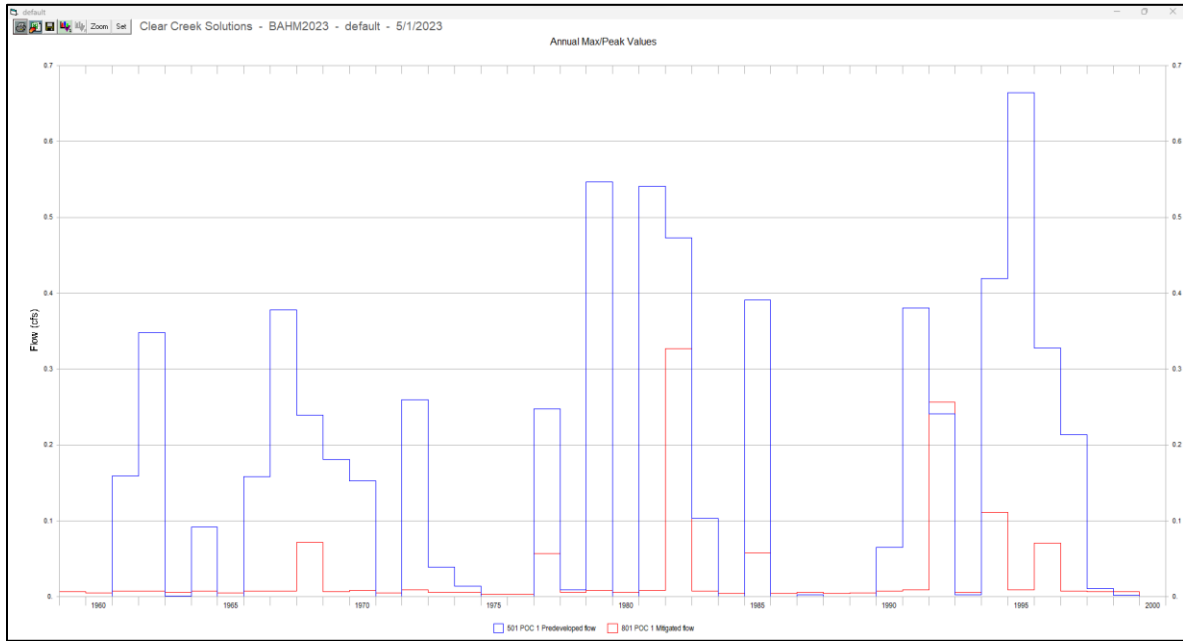

The hydrograph shows the yearly maximum/peak flow values for each time series for the entire simulation period (in this example, from water year 1960 through 2000).

The graph can be either saved or printed.

REPORTS SCREEN

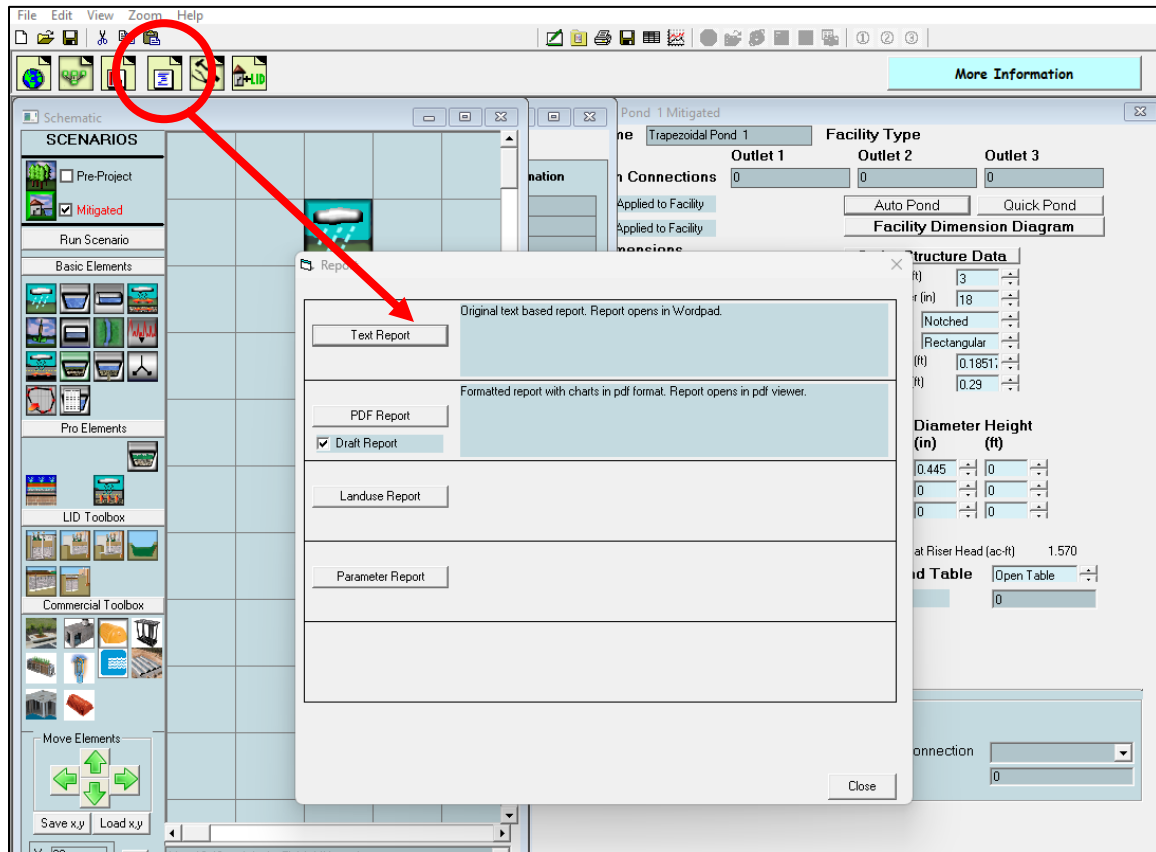

The Reports tool bar button (fourth from the left) brings up the Report screen where the user can look at all of the project input and output. The project report can be saved or printed.

The user has the option of producing the report file in a number of different formats.

Click on “Text Report” button to generate the report file in WordPad RTF format.

General Model Information


BAHM2023 Project Name: default
Site Name:
Site Address:
City:
Report Date: 5/1/2023
Gage: San Jose
Data Start: 1959/10/01
Data End: 2000/09/30
Timestep: Hourly
Precip Scale: 0.862
Version Date: 2023/04/26

POC Thresholds


Low Flow Threshold for POC1:	10 Percent of the 2 Year
High Flow Threshold for POC1:	10 Year

DRAFT


You can view all the parts of the report in a PDF viewer.

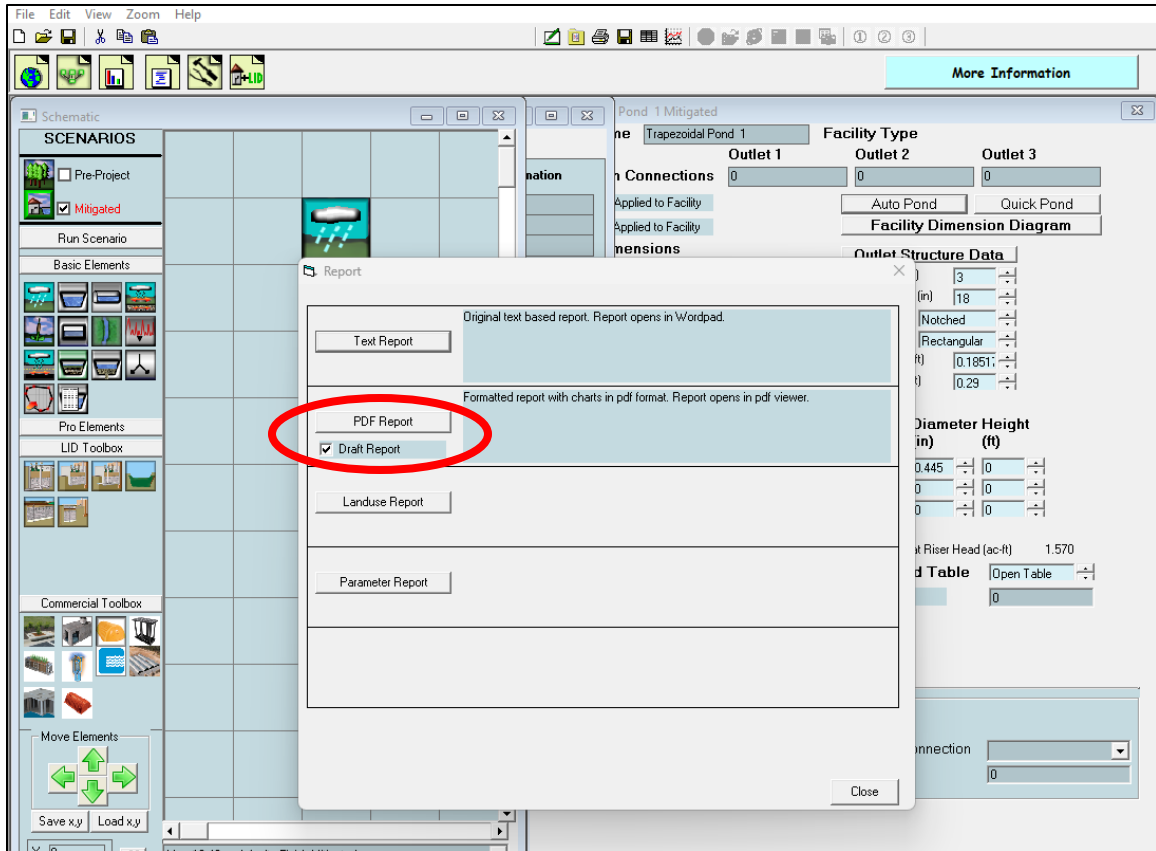

Click on “PDF Report” button to generate the report file in PDF format.

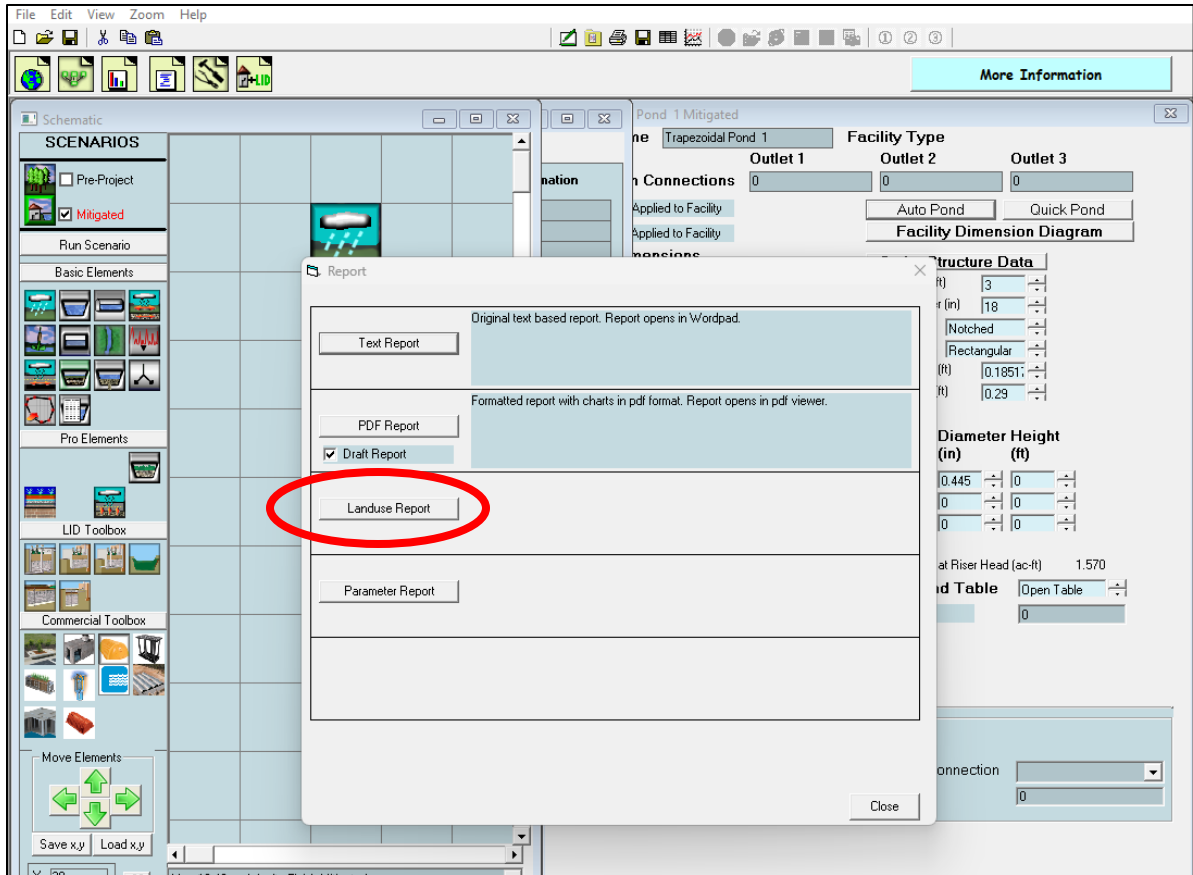


Click on “Landuse Report” button to generate a listing of the input basin land use data in WordPad RTF format.

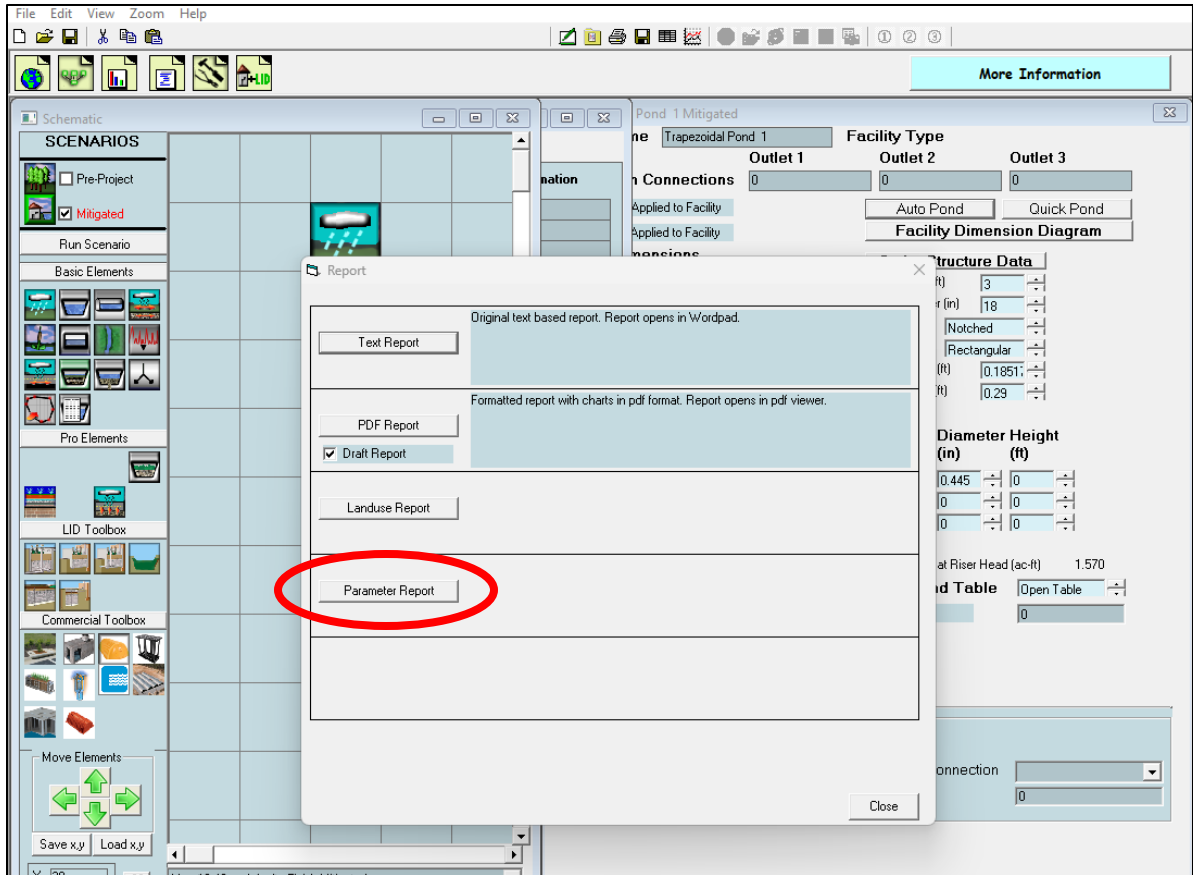

Click on “Parameter Report” button to generate a listing of the HSPF input parameter values that have been changed from their default values. The listing is in WordPad RTF format. If the listing is blank, then there have been no HSPF input parameter value changes made.

Learn more about BAHM2023 Reports here:
www.clearcreeksolutions.info/bahm-course-home


TOOLS SCREEN

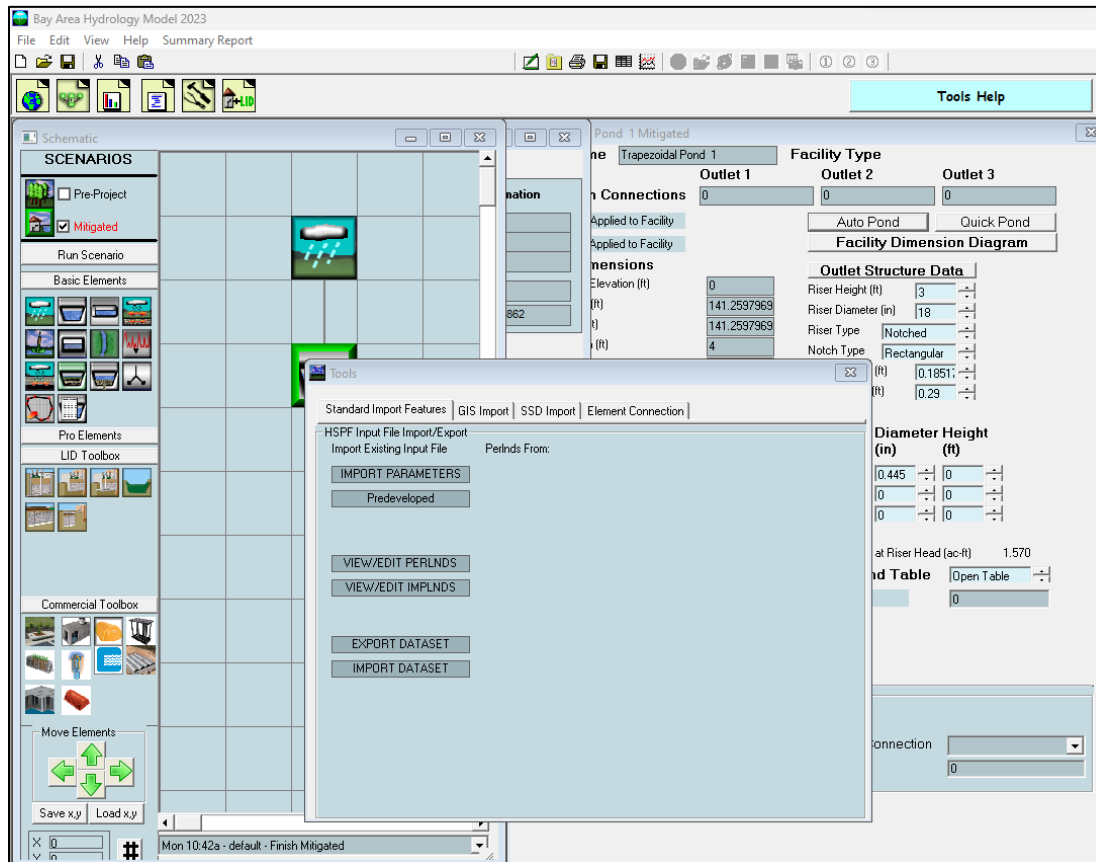

The Tools screen is accessed with the Tools tool bar (second from the right). The two purposes of the Tools screen are:

- (1) To allow users to import HSPF PERLND parameter values from existing HSPF UCI files and/or view and edit BAHM2023 PERLND parameter values.
- (2) To allow users to export time series datasets.

To export a time series dataset, click on the Export Dataset box.

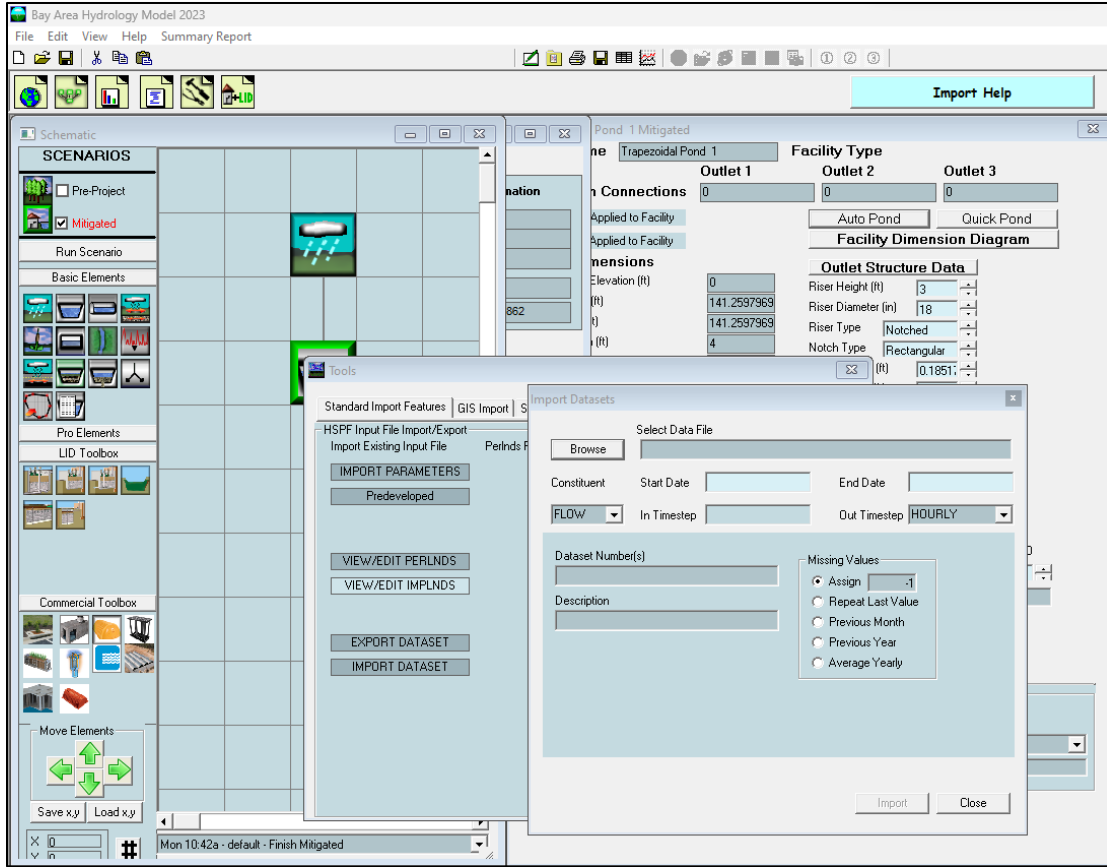


The list of available time series datasets will be shown. The user can select the start and end dates for the data they want to export.

The time step (hourly, daily, monthly, yearly) can also be specified. If the user wants daily, monthly, or yearly data, the user is given the choice of either selecting the maximum, minimum, or the sum of the hourly values.


Click the Export button.

The user provides a file name and the format or type of file. The file type can be ASCII, comma delimited, Excel spreadsheet, or Access database.

Click Save to save the exported time series file.

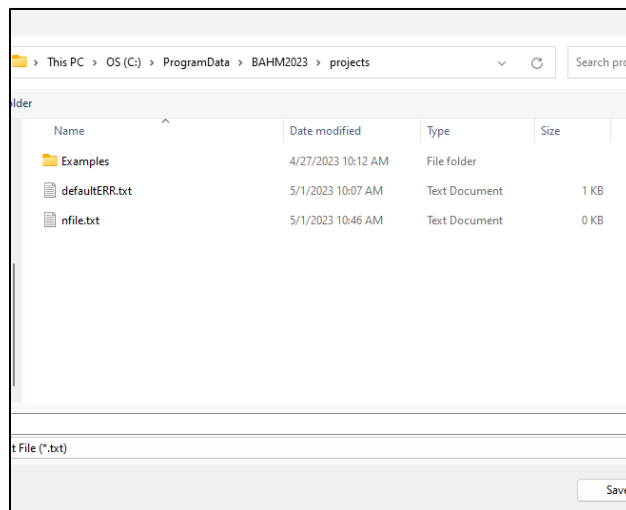


LID ANALYSIS SCREEN

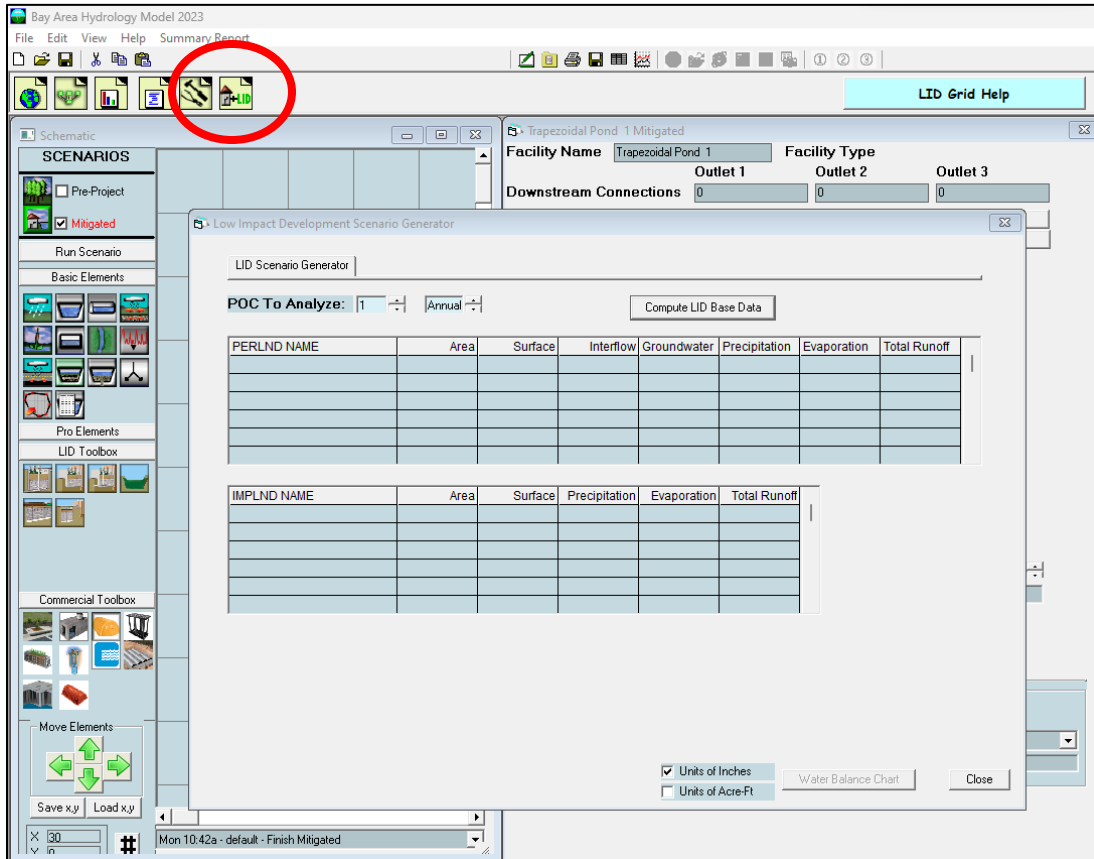

The LID tool bar button (farthest on the right) brings up the Low Impact Development Scenario Generator screen.

The LID scenario generator can be used to compare the amount of runoff from different land types and combinations. The user can quickly see how changing the land use affects surface runoff, interflow, groundwater, and evapotranspiration.

NOTE: The LID scenario generator works only in the Mitigated scenario.

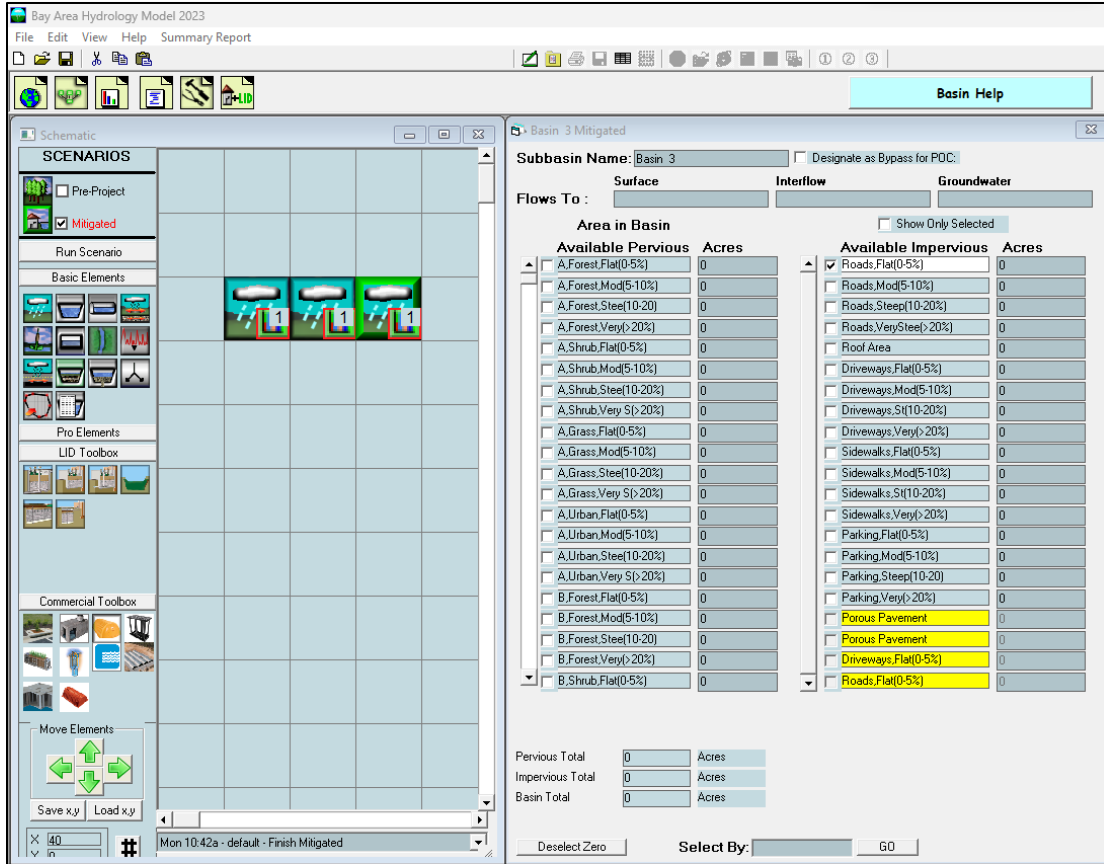

The easiest way to compare different land use scenarios is to place all of them on the same Schematic Editor screen grid. Each basin can then represent a different land use scenario. Because the LID scenario generator only compares runoff volume, there is no need to do any routing through a conveyance system or stormwater facility.


For this example, the three basins are assigned the following land uses:

Basin 1: 100 acres C/D, Shrub, Flat

Basin 2: 100 acres C/D, Urban, Flat


Basin 3: 50 acres C/D, Urban, Flat; 50 acres Parking Flat

Each basin is assigned a different POC (point of compliance) for the LID analysis.

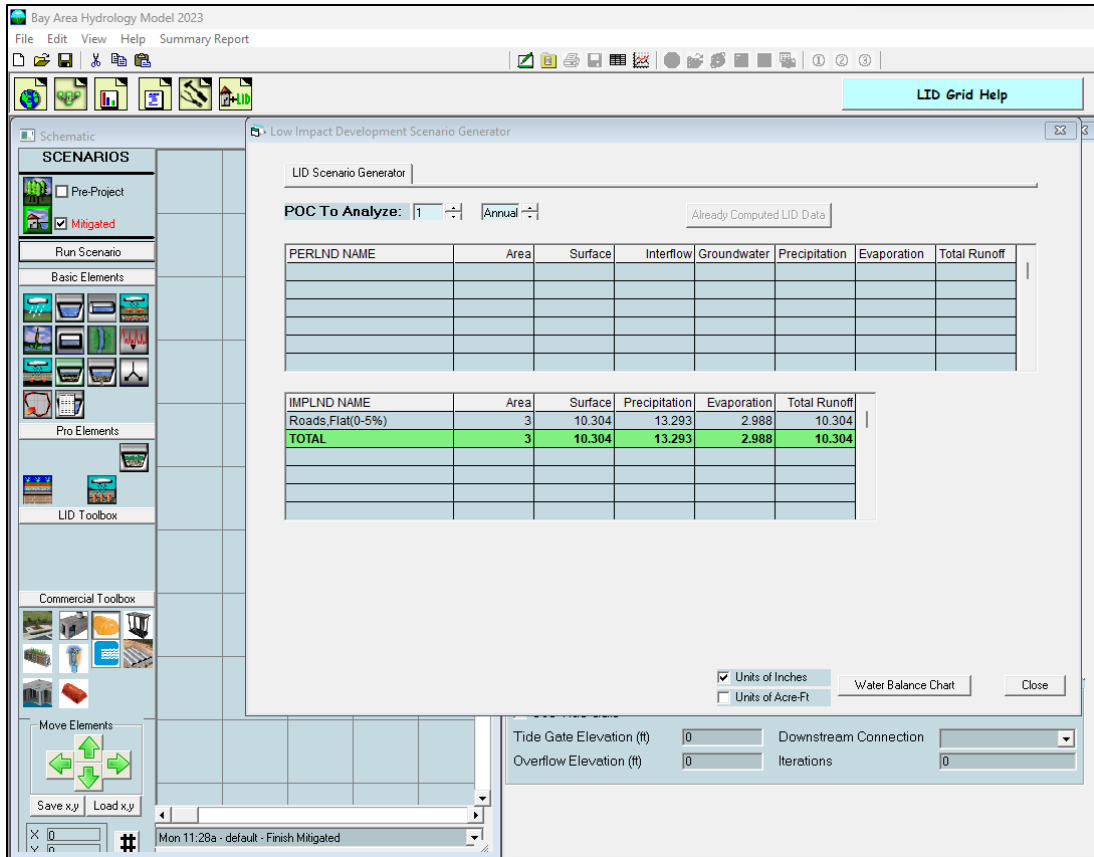

Click on the Compute LID Base Data button to generate the LID analysis data and summarize the surface runoff, interflow, groundwater, precipitation, evaporation, and total runoff for all of the basins. The results will be shown for each basin in terms of its POC.

Bay Area Hydrology Model 2023 User Manual – December 2023

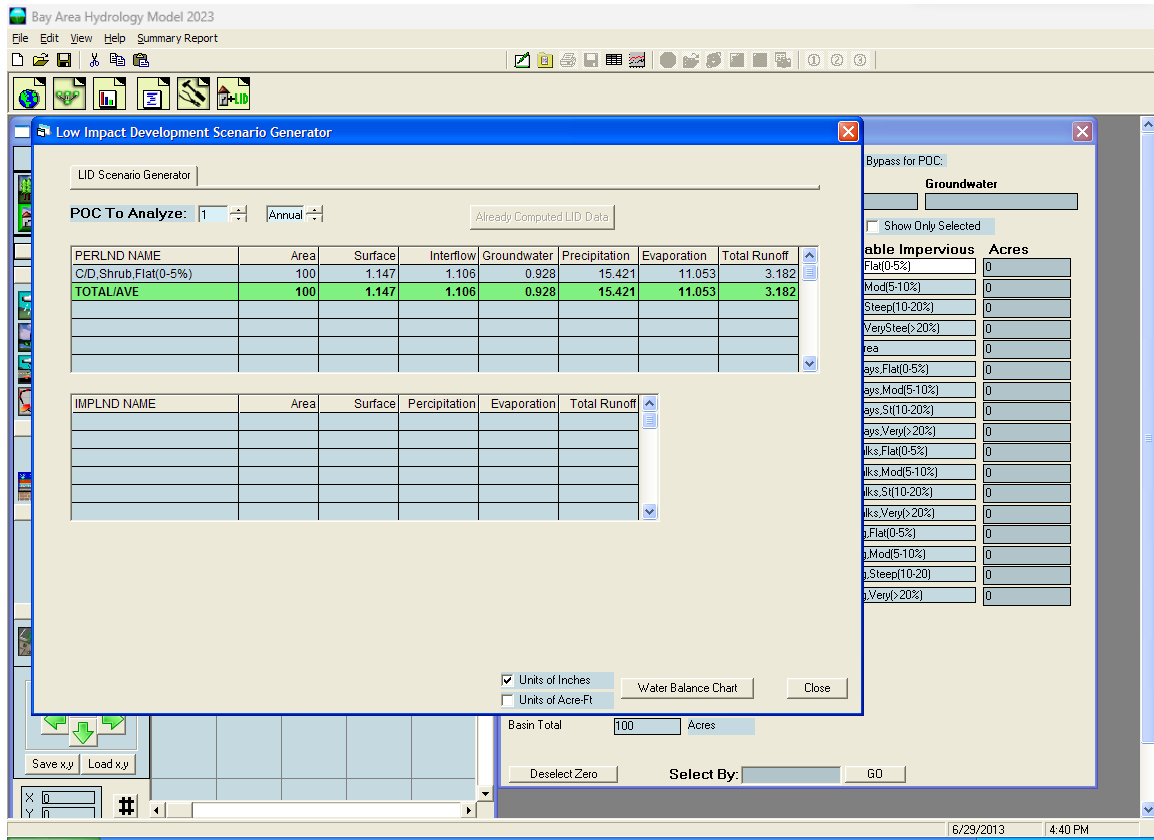

For Basin 1 (50 acres of C/D, Shrub, Flat), the distribution of the precipitation is:
 Surface runoff = 1.147 inches per year
 Interflow = 1.106 inches per year
 Groundwater = 0.928 inches per year
 Evaporation = 11.053 inches per year


The sum of the surface runoff + interflow + groundwater + evaporation equals 14.234 inches per year. The precipitation at this site equals 15.421 inches per year. The difference is the water that goes to deep or inactive groundwater and is not available to the downstream stream system.

Note that, for basins with the Urban land use category, irrigation will increase surface runoff, interflow, groundwater, and evaporation and the total will be greater than the precipitation because of the additional irrigation water.

To look at the other basins, click on the Select POC To arrow and select the basin of interest.

The LID analysis results can be presented in terms of either inches per year or acre-feet per year by checking the appropriate box in the lower right portion of the LID analysis screen.

To compare the different scenarios side-by-side in a graphical format click on the Water Balance Chart button.

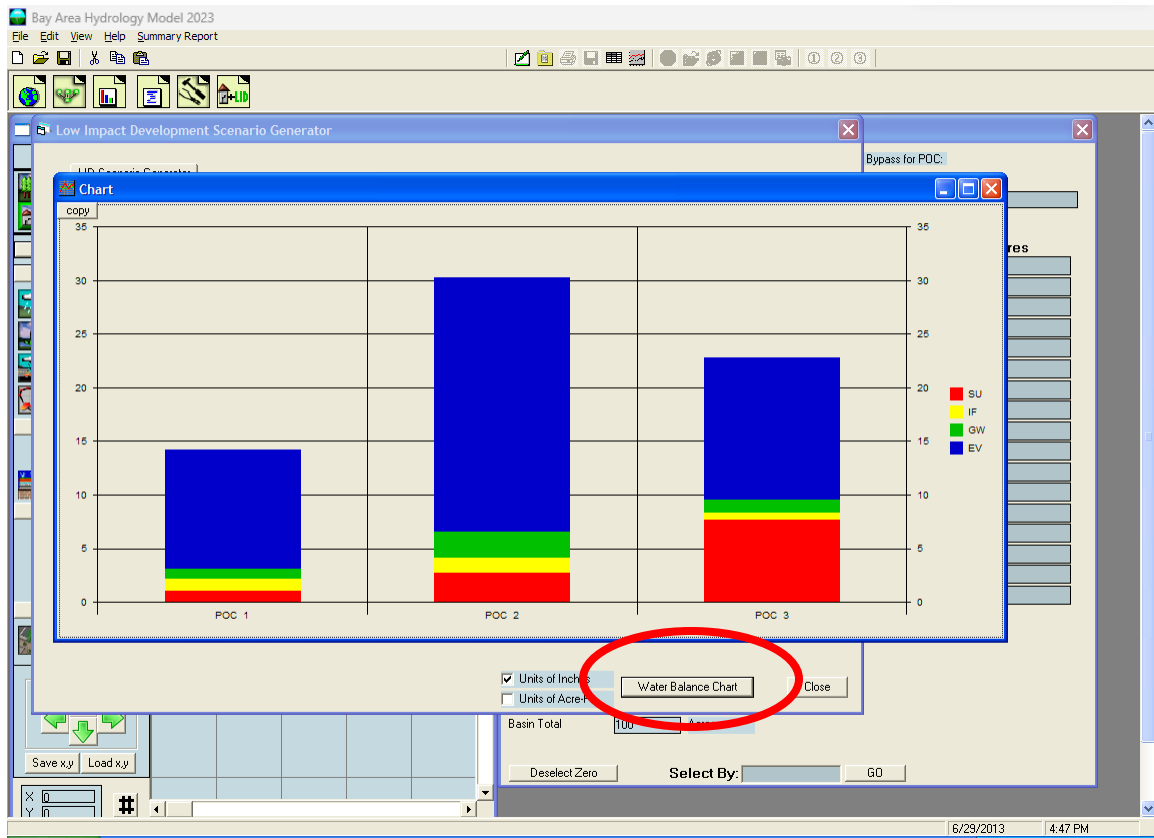


The water balance chart graphically displays the runoff distribution for all three land use scenarios side-by-side.

The bottom red is the surface runoff. Above in yellow is interflow; then green for groundwater and blue for evaporation. Basin 1 (Scenario 1) is all shrub vegetation and produces the least amount of surface runoff and interflow (the sum of surface and interflow is the total stormwater runoff). Basin 2 is all urban vegetation; it produces more surface runoff and interflow than Basin 1. Basin 3 is 50% urban vegetation and 50% impervious and produces the largest amount of surface runoff and interflow and smaller amounts of groundwater and evaporation.

A maximum of seven scenarios can be graphed at one time.

Learn more about LID Analysis here:
www.clearcreeksolutions.info/bahm-course-home

OPTIONS

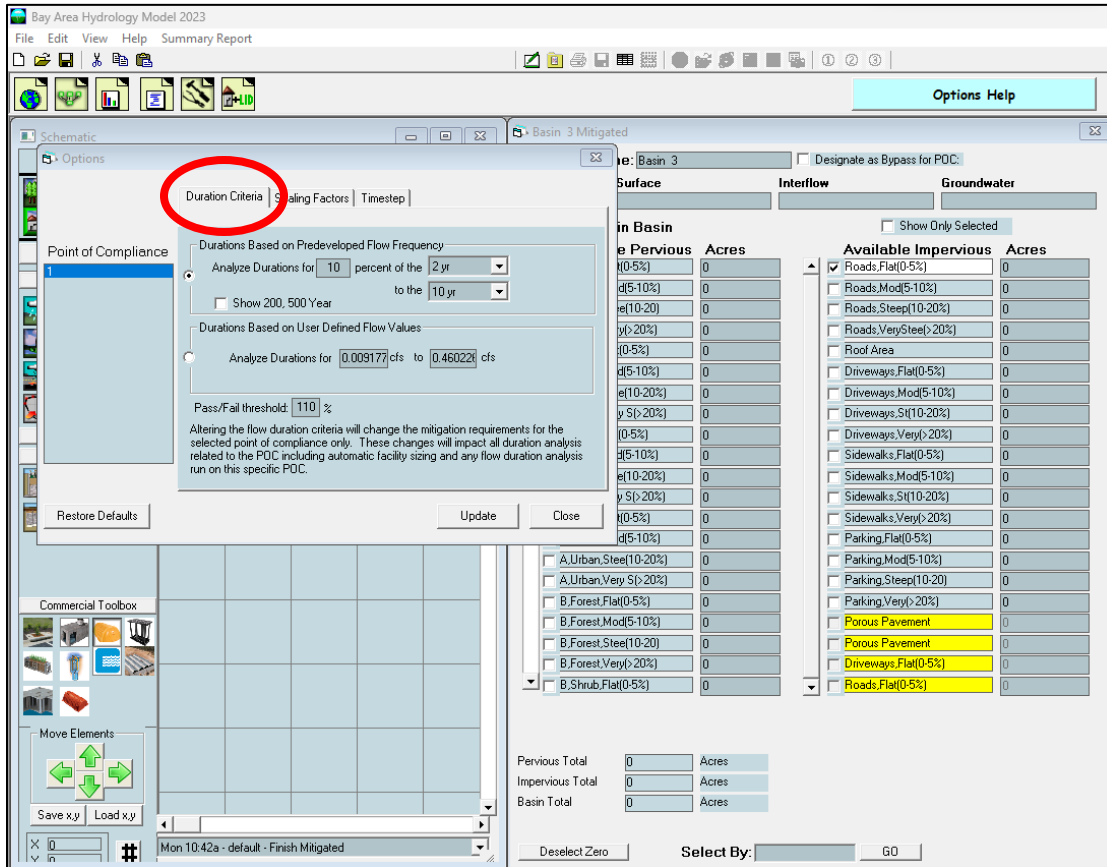

Options can be accessed by going to View, Options. This will bring up the Options screen and the ability to modify the built-in default duration criteria for flow duration matching and scaling factors for climate variables.

DURATION CRITERIA

The flow duration criteria are:

1. If the post-development flow duration values exceed any of the pre-project flow levels between 10% of the two-year and 100% of the ten-year pre-project peak flow values more than 10 percent of the time (110 Percent Threshold) then the flow duration standard has not been met.
2. If more than 10 percent of the flow duration levels exceed the 100 percent threshold then the flow duration standard has not been met.

The duration criteria in BAHM2023 can be modified by the user if appropriate and the local municipal permitting agency allows (see NOTE below).

The user can conduct the duration analysis using either (1) durations based on Pre-project flow frequency, or (2) durations based on user defined flow values.

If using durations based on Pre-project flow frequency, the percent of the lower limit can be changed from the default of the 2-year flow event to a higher or lower percent value. The lower and upper flow frequency limits (2-year and 10-year) also can be changed.

If using durations based on user defined flow values, click on that option and input the lower and upper flow values.


The default pass/fail threshold is 110%. This value can be changed by the user.

The duration criteria can be changed for a single point of compliance. Click on the Update button once all of the changes have been made. To return to the default values click on the Restore Defaults button.

NOTE: Any change(s) to the default duration criteria must be approved by the appropriate local municipal permitting agency or specified in Appendix D.

Learn more about Duration Criteria here:
www.clearcreeksolutions.info/bahm-course-home

SCALING FACTORS

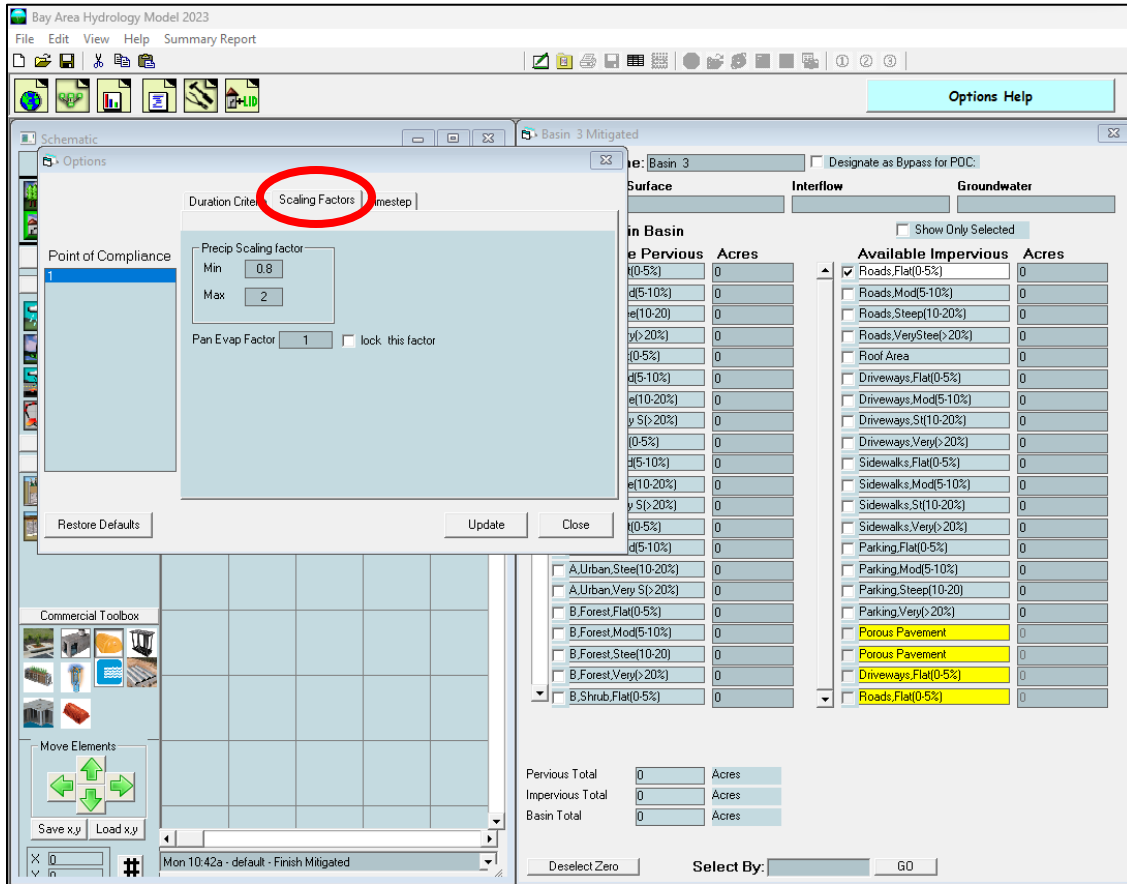


The user can change the scaling factors for precipitation (minimum and maximum) and pan evaporation.

NOTE: Any change in default scaling factors requires approval by the local municipal permitting agency or Appendix D.

Click on the Update button once all of the changes have been made. To return to the default values, click on the Restore Defaults button.

TIMESTEP

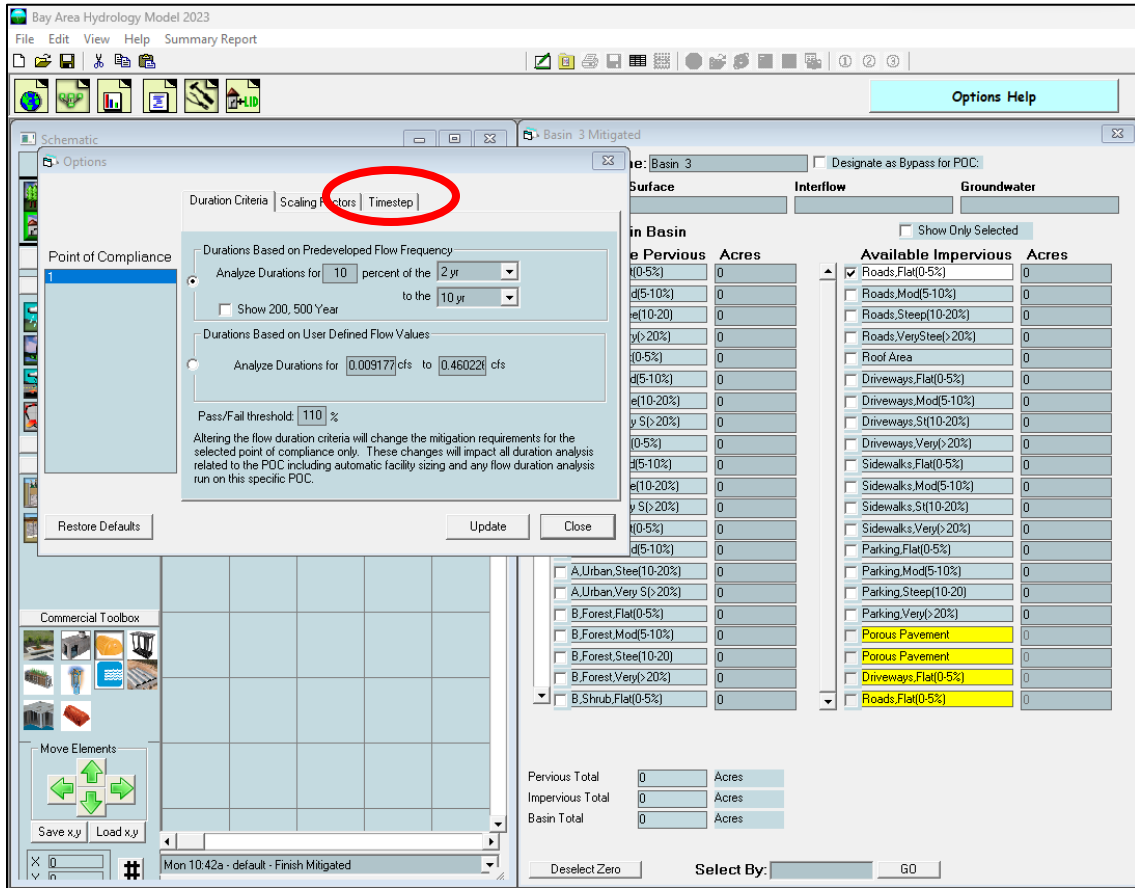


The user can change the time step for the HSPF calculations. The default time step is hourly.

NOTE: Any change in the default time step requires approval by the local municipal permitting agency or Appendix D.


Click on the Update button a change has been made. To return to the default value, click on the Restore Defaults button.

REPORT

When a BAHM 2023 report is rendered, the default is to output the report in PDF format. The first page seen in the report is the title page, indicating that this document is BAHM2023 project report.

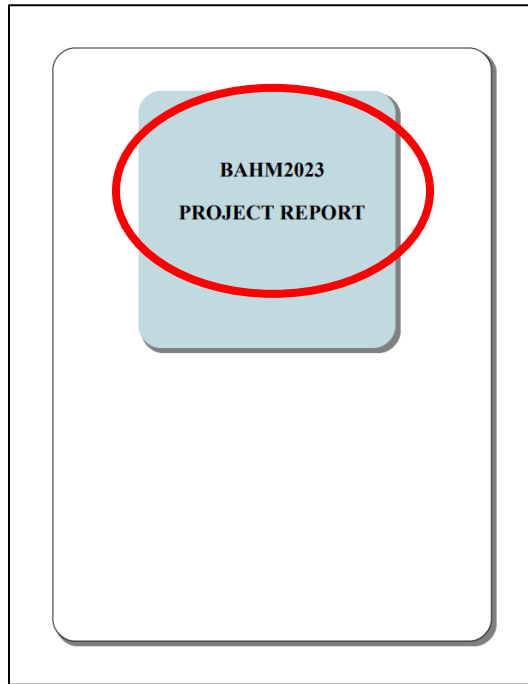

The user can determine whether the report will contain a “Draft” watermark on every page. Unselect this feature to remove the watermark before initiating the report rendering process.

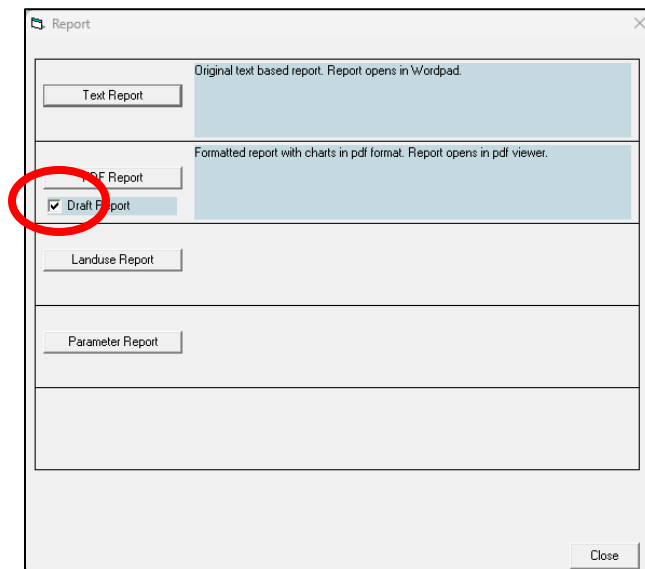

This page shows the general model information, including the user entered site name, address, and city. The gage that was utilized, as well as the precipitation scale are important parameters to note.

General Model Information
BAHM2023 Project Name: BAHM User Test Project
Site Name:
Site Address:
City:
Report Date: 5/19/2023
Gage: LIVERMORE
Data Start: 1959/10/01
Data End: 2004/09/30
Timestep: Hourly
Precip Scale: 1.333
Version Date: 2023/04/26

POC Thresholds

Low Flow Threshold for POC1:	10 Percent of the 2 Year
High Flow Threshold for POC1:	10 Year


Next, the report will show all predeveloped landuse basins and their corresponding areas.

Landuse Basin Data
Predeveloped Land Use


Basin 1

Bypass:	No
GroundWater:	No
Pervious Land Use C D,Forest,Flat(0-5)	acre 3
Pervious Total	3
Impervious Land Use	acre
Impervious Total	0
Basin Total	3

If routing is present in the predeveloped scenario, it will be noted in this section.

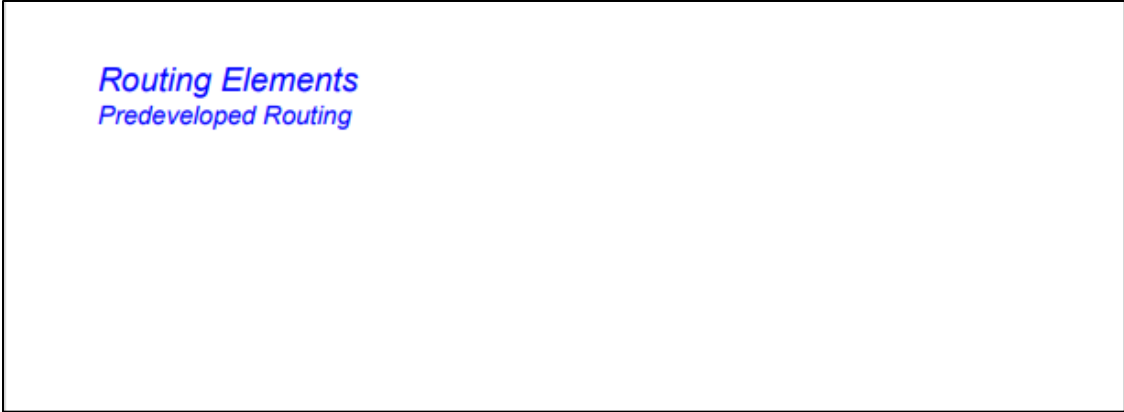

Mitigated routing is noted in this section. In addition, mitigation facility parameters can be seen below the facility name. This includes dimensions, outlets, facility type, and any other pertinent parameters.

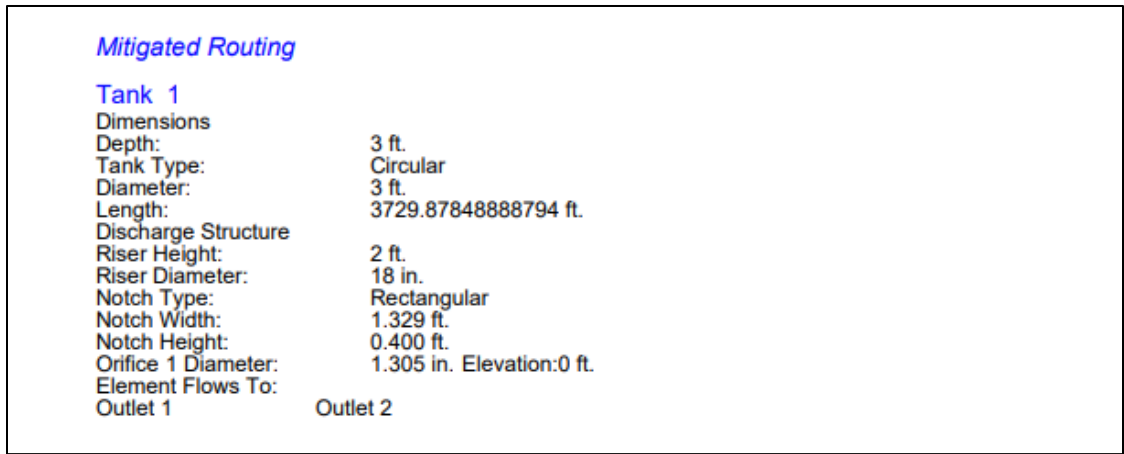

A stage-storage-discharge relationship can be seen for all project mitigation facilities.

Stage(feet)	Area(ac.)	Volume(ac-ft.)	Discharge(cfs)	Infiltr(cfs)
0.0000	0.000	0.000	0.000	0.000
0.0333	0.053	0.001	0.008	0.000
0.0667	0.075	0.003	0.011	0.000
0.1000	0.092	0.006	0.014	0.000
0.1333	0.105	0.009	0.016	0.000
0.1667	0.117	0.013	0.018	0.000
0.2000	0.128	0.017	0.020	0.000
0.2333	0.137	0.021	0.022	0.000
0.2667	0.146	0.026	0.023	0.000
0.3000	0.154	0.031	0.025	0.000
0.3333	0.161	0.036	0.026	0.000
0.3667	0.168	0.042	0.028	0.000
0.4000	0.174	0.048	0.029	0.000
0.4333	0.180	0.053	0.030	0.000
0.4667	0.186	0.060	0.031	0.000
0.5000	0.191	0.066	0.032	0.000
0.5333	0.196	0.072	0.033	0.000
0.5667	0.201	0.079	0.034	0.000
0.6000	0.205	0.086	0.035	0.000
0.6333	0.209	0.093	0.036	0.000
0.6667	0.213	0.100	0.037	0.000
0.7000	0.217	0.107	0.038	0.000
0.7333	0.220	0.114	0.039	0.000

Analysis results for all points of compliance can be seen with an accompanying flow duration and frequency graph for the predeveloped and mitigated scenarios.

Year	Predeveloped	Mitigated
1960	0.584	0.309
1961	0.283	0.058
1962	0.515	0.314
1963	0.839	1.019
1964	0.074	0.727
1965	0.416	0.544
1966	0.359	0.190
1967	2.511	2.548
1968	0.652	0.818
1969	1.149	0.740
1970	0.817	0.469
1971	0.651	0.789
1972	0.003	0.287
1973	1.731	1.064

A summary of landuse totals and flow frequency measurements can be found in this section.


Predeveloped Landuse Totals for POC #1	
Total Pervious Area:	3
Total Impervious Area:	0
Mitigated Landuse Totals for POC #1	
Total Pervious Area:	0
Total Impervious Area:	3
Flow Frequency Method: Weibull	
Flow Frequency Return Periods for Predeveloped. POC #1	
Return Period	Flow(cfs)
2 year	0.594182
5 year	1.176324
10 year	1.568218
25 year	1.798659
Flow Frequency Return Periods for Mitigated. POC #1	
Return Period	Flow(cfs)
2 year	0.544344
5 year	0.979638
10 year	1.474068
25 year	1.730877

A summary of the Annual Peaks, ranked, can be seen in this section.

Ranked Annual Peaks
 Ranked Annual Peaks for Predeveloped and Mitigated. POC #1

Rank	Predeveloped	Mitigated
1	2.5106	2.5479
2	1.7309	1.6531
3	1.5802	1.6280
4	1.5801	1.5692
5	1.5619	1.4233
6	1.5197	1.1093
7	1.4829	1.0889
8	1.3312	1.0640
9	1.1839	1.0192
10	1.1492	0.8371
11	1.0135	0.8288
12	0.9538	0.8180
13	0.8974	0.8080
14	0.8843	0.7887
15	0.8391	0.7402
16	0.8171	0.7268
17	0.7843	0.7265
18	0.7694	0.6873


A brief analysis result of the project’s points of compliance, and flow duration table can be seen below.

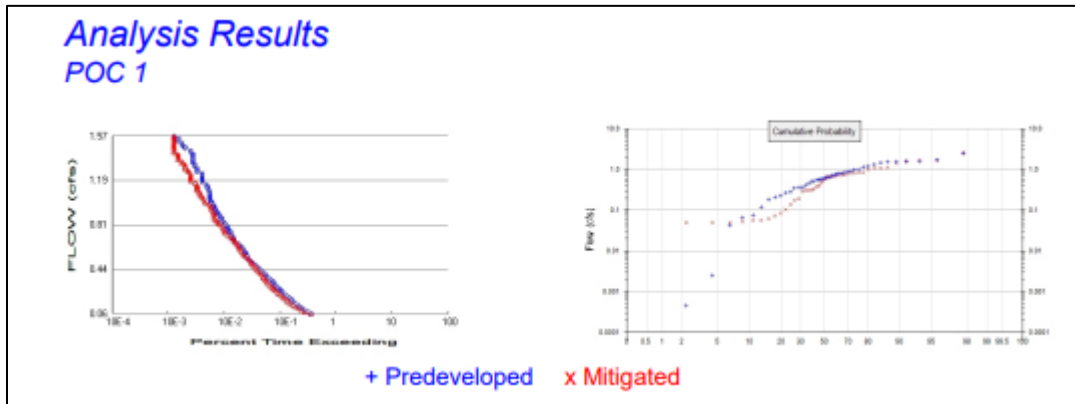


Duration Flows
 The Facility PASSED

Flow(cfs)	Predev	Mit	Percentage	Pass/Fail
0.0594	1431	1399	97	Pass
0.0747	1260	1117	88	Pass
0.0899	1105	962	87	Pass
0.1051	976	836	85	Pass
0.1204	878	742	84	Pass
0.1356	802	670	83	Pass
0.1509	729	597	81	Pass
0.1661	676	547	80	Pass
0.1813	627	499	79	Pass
0.1966	572	458	80	Pass
0.2118	520	421	80	Pass
0.2271	480	383	79	Pass
0.2423	439	356	81	Pass
0.2575	411	326	79	Pass

The schematic for the entire pre-project scenario can be seen next.

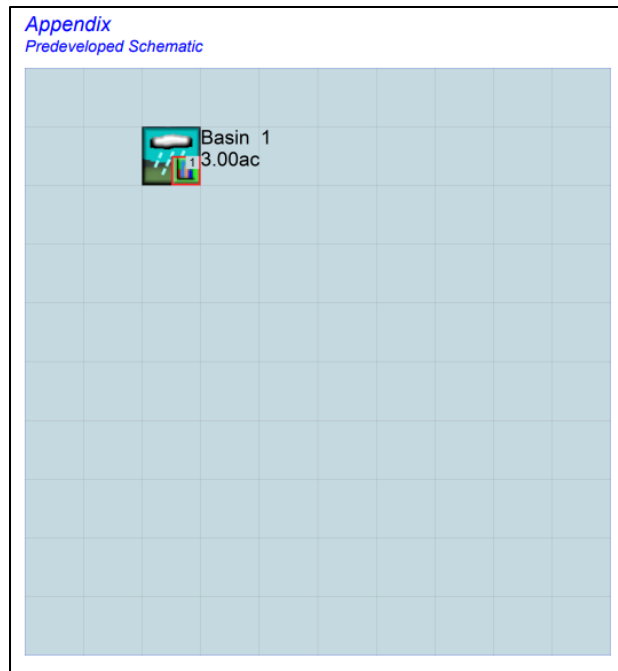

The schematic for the entire mitigated scenario can be seen next.

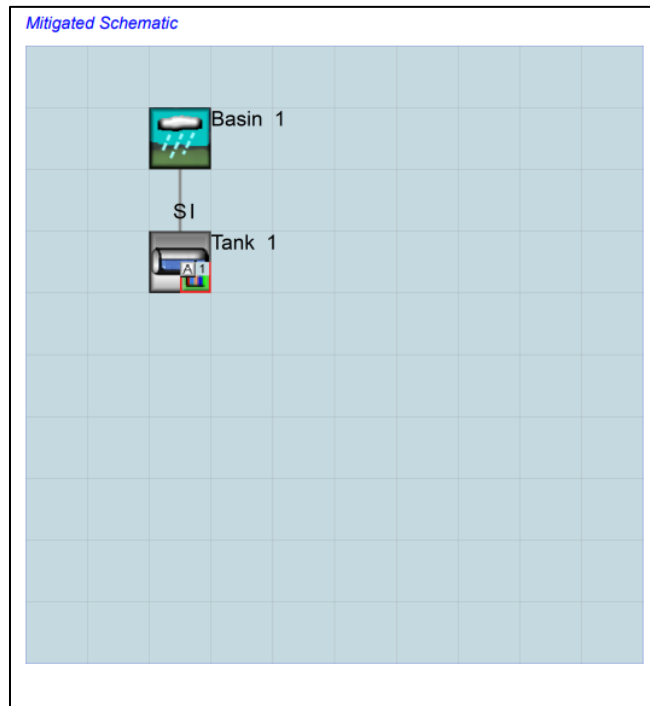

If there were any changes to the model defaults, such as PERLND and IMPLND modifications, they will be listed here.

Model Default Modifications

Total of 0 changes have been made.

PERLND Changes
No PERLND changes have been made.

IMPLND Changes
No IMPLND changes have been made.

The UCI file for the entire project can be seen in this section.


```
Predeveloped UCI File
RUN
GLOBAL
  WWHM4 model simulation
  START 1959 10 01      END 2004 09 30
  RUN INTERP OUTPUT LEVEL 3 0
  RESUME 0 RUN 1      UNIT SYSTEM 1
END GLOBAL

FILES
<File> <Un#> <-----File Name----->***
<-ID->
WDM 26 BAHM User Test Project.wdm
MESSU 25 PreBAHM User Test Project.MES
27 PreBAHM User Test Project.L61
28 PreBAHM User Test Project.L62
30 POCSAHM User Test Project1.dat
END FILES


OPN SEQUENCE
INGRP INDELT 00:60
  PERLND 33
  COPY 501
  DISPLY 1
END INGRP
END OPN SEQUENCE
DISPLY
DISPLY-INFO1
# - #<-----Title----->***TRAN PIVL DIG1 FIL1 PYR DIG2 FIL2 YRND
1 Basin 1 MAX 1 2 30 9
END DISPLY-INFO1
END DISPLY
COPY
```

REVIEWER CHECKLIST

Provided in BAHM2023 is a reviewer checklist that allows reviewers to evaluate submitted projects in an ordered and thorough manner. To utilize the reviewer checklist, the .WHM file must be provided by the developer’s engineer in order to run BAHM 2023. The reviewer checklist steps are as follows:

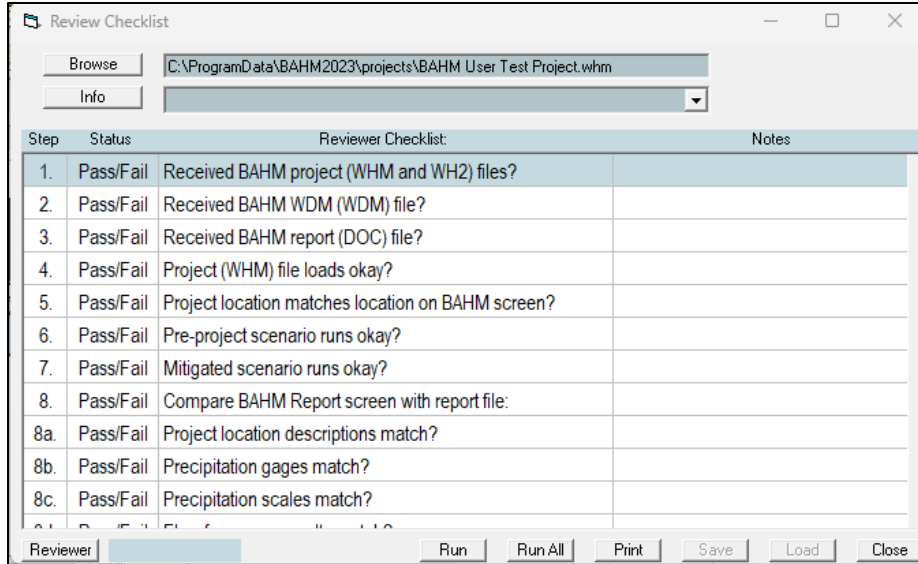

First, reviewers can enter their information in the form seen below. This allows developers to track who reviewed their project and the date the reviewed occurred.

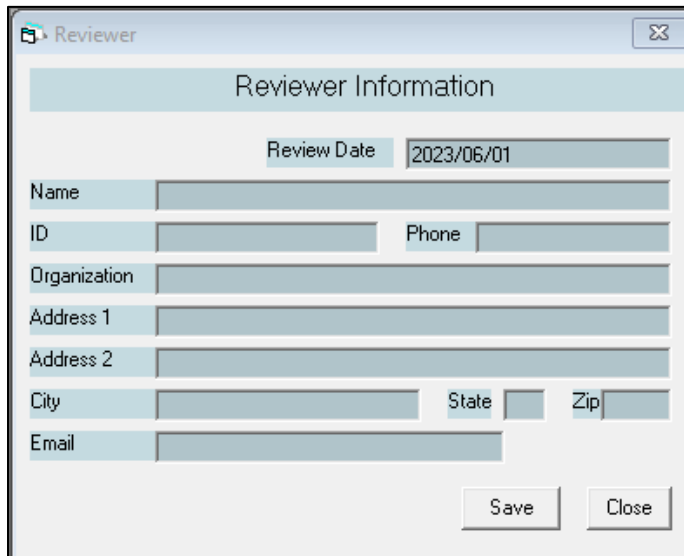

The reviewer checklist outlines 18 steps to reviewing a project. The program follows this progression checking for each parameter.

Step	Status	Reviewer Checklist:	Notes
1.	Pass/Fail	Received BAHM project (WHM and WH2) files?	
2.	Pass/Fail	Received BAHM WDM (WDM) file?	
3.	Pass/Fail	Received BAHM report (DOC) file?	
4.	Pass/Fail	Project (WHM) file loads okay?	
5.	Pass/Fail	Project location matches location on BAHM screen?	
6.	Pass/Fail	Pre-project scenario runs okay?	
7.	Pass/Fail	Mitigated scenario runs okay?	
8.	Pass/Fail	Compare BAHM Report screen with report file:	
8a.	Pass/Fail	Project location descriptions match?	
8b.	Pass/Fail	Precipitation gages match?	
8c.	Pass/Fail	Precipitation scales match?	
8d.	Pass/Fail	Flow frequency results match?	
8e.	Pass/Fail	All flow duration values PASS?	
8f.	Pass/Fail	Any pervious (PERLND) land use changes?	
8g.	Pass/Fail	Any impervious (IMPLND) land use changes?	
8h.	Pass/Fail	Any scaling factor changes?	
8i.	Pass/Fail	Any duration criteria changes?	
8j.	Pass/Fail	pond dimensions match?	
8k.	Pass/Fail	pond outlet structure info matches?	
9.	Pass/Fail	BAHM pond dimensions match drawings?	
10.	Pass/Fail	Infiltration set to YES for infiltration pond?	
11.	Pass/Fail	Total BAHM drainage area matches drainage maps/drawing?	
12.	Pass/Fail	Mitigated drainage area(s) match Pre-project?	
13.	Pass/Fail	Pre-project vegetation correct?	
14.	Pass/Fail	Mitigated land use areas correct?	
15.	Pass/Fail	Routing correct?	
16.	Pass/Fail	Check facility drawdown (if included):	
16a.	Pass/Fail	Used POC Mitigated stage?	
16b.	Pass/Fail	Drawdown times okay?	
17.	Pass/Fail	Options set to default values?	
18.	Pass/Fail	Other issues?	


“Browse” allows for the user to select a specific review.

“Info” provides additional information about the review.

Step 1: Indicates whether the reviewer received WHM and WH2 files. These files are the project files for any BAHM 2023 project.


Step 2: Indicates whether the reviewer received the BAHM WDM file. This is the database file needed to run the BAHM project.

Step 3: Asks if the reviewer received a BAHM report in document format. This report documented can be created in BAHM 2023 in draft or final format (typically in PDF format).

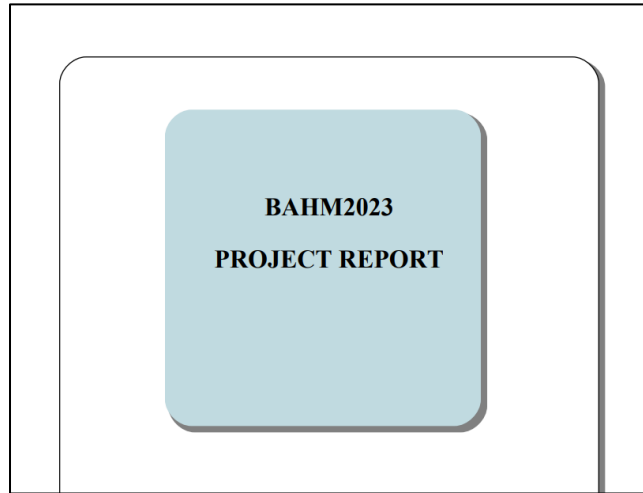

Step 4: Does the WHM file load properly? This file is needed to run and evaluate the project.


Step 5: Does the project location match the location seen in the project screen? The gage must be the same to duplicate the project results.

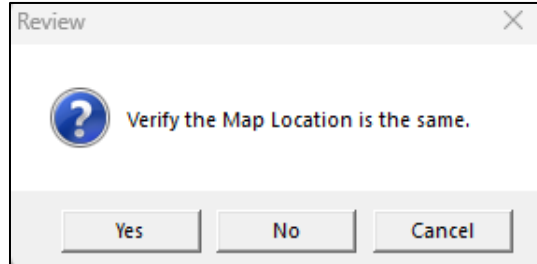


Step 6: The Pre-Project scenario runs properly? This will be needed to generate pre-project runoff and data.

Step 7: The Mitigated scenario runs properly? This will be needed to generate mitigated runoff data and evaluate facility performance.


Step 8a: Do the project location descriptions match? Locations will need to be the same for gage data.

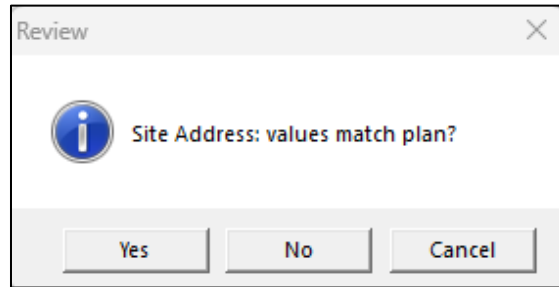


Step 8b: Do the precipitation gages match? These will need to be the same to duplicate project results.

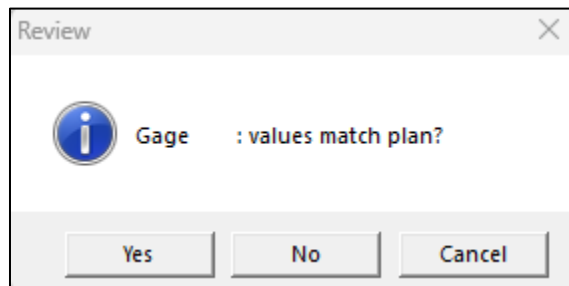


Step 8c: Scale factors need to match for the selected gage.

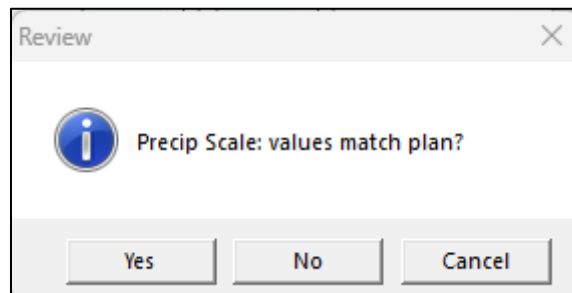

Step 8d: The software checks to make sure flow frequency data matches.

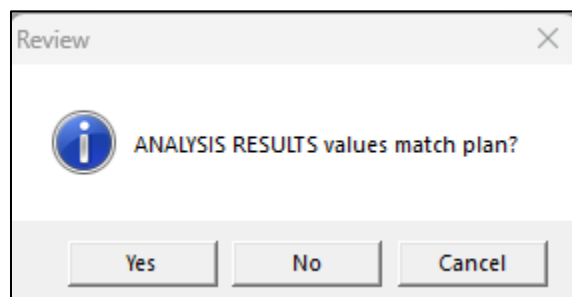


Step 8e: The software checks to make sure all flow frequency data passes.

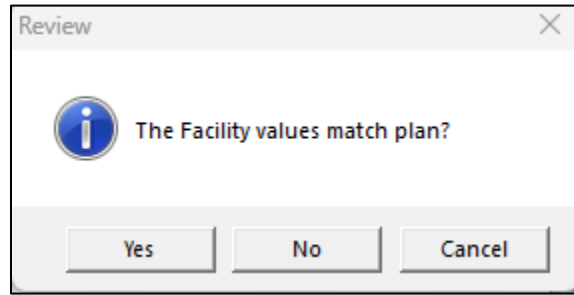


Step 8f: Any pervious (PERLND) land use changes? Landuse changes will modify project results.

Step 8g: Any impervious (IMPLND) land use changes? Landuse changes will modify project results.


Step 8h: Any scaling factor changes? Scaling factor modifications will change project results.

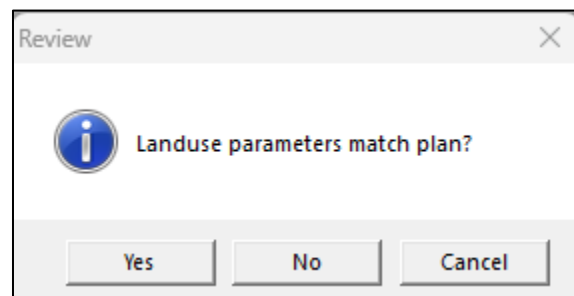

Step 8i: Any duration criteria changes? Duration criteria determines the pass/fail and flow duration curves.

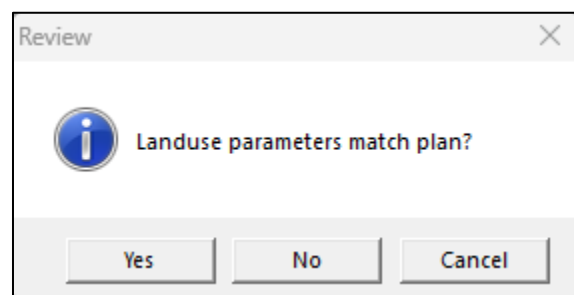


Step 8j: Do the pond dimensions match? This will affect facility performance.

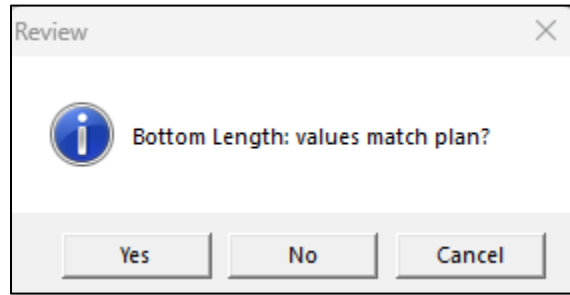


Step 8k: Do the outlets structures match? This will affect facility performance.



Step 9: Do the BAHM Pond dimensions match the drawing? These values need to be the same.

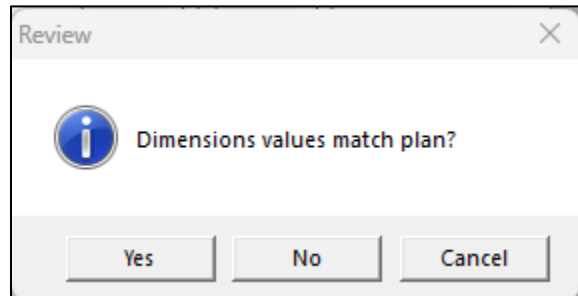

Step 10: Is infiltration set to YES for the infiltration pond?

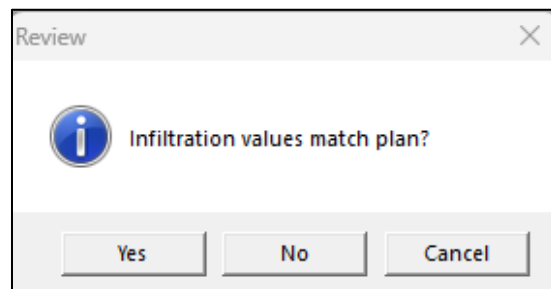

Step 11: Does the total BAHM drainage areas map plans/drawings?


Step 12: Mitigated drainage areas match pre-project? These areas need to match to verify results.

Step 13: Pre-project vegetation correct? Vegetation must be identical to duplicate results.

Step 14: Mitigated landuse areas correct? These must be identical to duplicate results.


Step 15: Routing correct? This will be needed to emulate project results.

Step 16: Check facility drawdown are included. Drawdown time cannot be exceeded in certain projects.

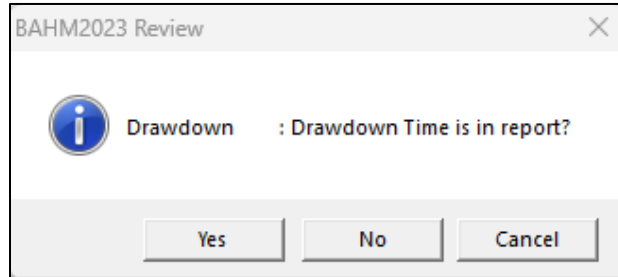

Step 16a: Used Point of Compliance in the mitigated stage? Point of Compliance is needed for analysis.

Step 16b: Drawdown times okay? Are the drawdown times acceptable for the project?

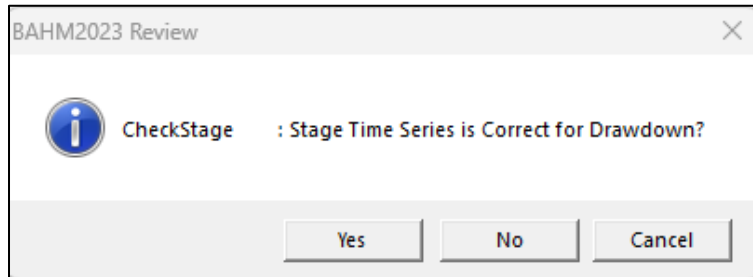

Step 17: Are the options set to default values?

Step 18: Any other project related issues of note?

Learn more about the Reviewer Checklist here:
www.clearcreeksolutions.info/bahm-course-home

APPENDIX A: DEFAULT BAHM2023 HSPF PERVIOUS PARAMETER VALUES FOR ALAMEDA, SAN MATEO AND CONTRA COSTA COUNTIES

The default BAHM2023 HSPF pervious parameter values are found in BAHM2023 file defaultpers.uci. These pervious parameter values have not changed from the original BAHM values.

The default BAHM2023 HSPF pervious parameter values for Alameda, San Mateo, and Contra Costa counties are based on HSPF calibrations of Castro Valley Creek and Alameda Creek. The default BAHM2023 HSPF pervious parameter values for Santa Clara County are based on the HSPF calibration of Ross Creek and Thompson Creek and are listed in Appendix B.

HSPF calibrations of Castro Valley Creek and Alameda Creek are documented in the report:

AQUA TERRA Consultants. 2006. Hydrologic Modeling of the Castro Valley Creek and Alameda Creek Watersheds with the U.S. EPA Hydrologic Simulation Program – FORTRAN (HSPF). Prepared for Alameda Countywide Clean Water Program. January 20, 2006.

Any changes in the default BAHM2023 HSPF pervious and impervious parameter values require approval by the local municipal permitting agency, unless covered by additional guidance in Appendix D.

HSPF parameter documentation is found in the document:

Bicknell, B.R., J.C. Imhoff, J.L. Kittle Jr, T.H. Jobes, and A.S. Donigian Jr. 2001. Hydrological Simulation Program – Fortran, User's Manual for Version 12. AQUA TERRA Consultants. Mountain View, CA.

Table 1. BAHM2023 Alameda/San Mateo/Contra Costa Pervious Land Types

PERLND No.	Soil	Vegetation/Surface	Slope
1	A	Forest	Flat(0-5%)
2	A	Forest	Moderate(5-10%)
3	A	Forest	Steep(10-20%)
4	A	Forest	Very Steep(>20%)
5	A	Shrub	Flat(0-5%)
6	A	Shrub	Moderate(5-10%)
7	A	Shrub	Steep(10-20%)
8	A	Shrub	Very Steep(>20%)
9	A	Grass	Flat(0-5%)
10	A	Grass	Moderate(5-10%)
11	A	Grass	Steep(10-20%)
12	A	Grass	Very Steep(>20%)
13	A	Urban	Flat(0-5%)
14	A	Urban	Moderate(5-10%)
15	A	Urban	Steep(10-20%)
16	A	Urban	Very Steep(>20%)
17	B	Forest	Flat(0-5%)
18	B	Forest	Moderate(5-10%)
19	B	Forest	Steep(10-20%)
20	B	Forest	Very Steep(>20%)
21	B	Shrub	Flat(0-5%)
22	B	Shrub	Moderate(5-10%)
23	B	Shrub	Steep(10-20%)
24	B	Shrub	Very Steep(>20%)
25	B	Grass	Flat(0-5%)
26	B	Grass	Moderate(5-10%)
27	B	Grass	Steep(10-20%)
28	B	Grass	Very Steep(>20%)
29	B	Urban	Flat(0-5%)
30	B	Urban	Moderate(5-10%)
31	B	Urban	Steep(10-20%)
32	B	Urban	Very Steep(>20%)
33	C/D	Forest	Flat(0-5%)
34	C/D	Forest	Moderate(5-10%)
35	C/D	Forest	Steep(10-20%)
36	C/D	Forest	Very Steep(>20%)
37	C/D	Shrub	Flat(0-5%)
38	C/D	Shrub	Moderate(5-10%)
39	C/D	Shrub	Steep(10-20%)
40	C/D	Shrub	Very Steep(>20%)
41	C/D	Grass	Flat(0-5%)

42	C/D	Grass	Moderate(5-10%)
43	C/D	Grass	Steep(10-20%)
44	C/D	Grass	Very Steep(>20%)
45	C/D	Urban	Flat(0-5%)
46	C/D	Urban	Moderate(5-10%)
47	C/D	Urban	Steep(10-20%)
48	C/D	Urban	Very Steep(>20%)

Table 2. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values – Part I

PERLND No.	LZSN	INFILT	LSUR	SLSUR	KVARY	AGWRC
1	5.2	0.100	400	0.05	0.8	0.985
2	4.8	0.075	350	0.10	0.8	0.985
3	4.5	0.055	300	0.15	0.8	0.985
4	4.2	0.045	200	0.25	0.8	0.985
5	5.2	0.090	400	0.05	0.8	0.955
6	4.8	0.070	350	0.10	0.8	0.955
7	4.5	0.045	300	0.15	0.8	0.955
8	4.2	0.040	200	0.25	0.8	0.955
9	5.2	0.090	400	0.05	0.8	0.955
10	4.8	0.070	350	0.10	0.8	0.955
11	4.5	0.045	300	0.15	0.8	0.955
12	4.2	0.040	200	0.25	0.8	0.955
13	5.0	0.060	400	0.05	1.2	0.997
14	4.6	0.050	350	0.10	1.2	0.997
15	4.2	0.040	300	0.15	1.2	0.997
16	3.8	0.030	200	0.25	1.2	0.997
17	4.5	0.080	400	0.05	1.2	0.980
18	4.3	0.060	350	0.10	1.2	0.980
19	4.1	0.045	300	0.15	1.2	0.980
20	3.9	0.035	200	0.25	1.2	0.980
21	4.5	0.070	400	0.05	1.2	0.950
22	4.3	0.055	350	0.10	1.2	0.950
23	4.1	0.040	300	0.15	1.2	0.950
24	3.9	0.030	200	0.25	1.2	0.950
25	4.5	0.070	400	0.05	1.2	0.950
26	4.3	0.055	350	0.10	1.2	0.950
27	4.1	0.040	300	0.15	1.2	0.950
28	3.9	0.030	200	0.25	1.2	0.950
29	4.3	0.050	400	0.05	1.8	0.995
30	4.1	0.040	350	0.10	1.8	0.995
31	3.9	0.030	300	0.15	1.8	0.995
32	3.4	0.025	200	0.25	1.8	0.995
33	4.0	0.045	400	0.05	2.0	0.980
34	3.8	0.040	350	0.10	2.0	0.980
35	3.6	0.035	300	0.15	2.0	0.980
36	3.4	0.030	200	0.25	2.0	0.980
37	4.0	0.040	400	0.05	2.0	0.950
38	3.8	0.035	350	0.10	2.0	0.950
39	3.6	0.030	300	0.15	2.0	0.950
40	3.4	0.025	200	0.25	2.0	0.950
41	4.0	0.040	400	0.05	2.0	0.950
42	3.8	0.035	350	0.10	2.0	0.950
43	3.6	0.030	300	0.15	2.0	0.950
44	3.4	0.025	200	0.25	2.0	0.950

Bay Area Hydrology Model 2023 User Manual – December 2023

45	3.8	0.035	400	0.05	3.0	0.995
46	3.6	0.030	350	0.10	3.0	0.995
47	3.4	0.022	300	0.15	3.0	0.995
48	3.2	0.020	200	0.25	3.0	0.995

LZSN: Lower Zone Storage Nominal (inches)

INFILT: Infiltration (inches per hour)

LSUR: Length of surface flow path (feet)

SLSUR: Slope of surface flow path (feet/feet)

KVARY: Variable groundwater recession

AGWRC: Active Groundwater Recession Constant (per day)

Table 3. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values – Part II

PERLND No.	INFEXP	INFILD	DEEPPFR	BASETP	AGWETP
1	2	2	0.02	0	0
2	2	2	0.02	0	0
3	2	2	0.02	0	0
4	2	2	0.02	0	0
5	2	2	0.02	0	0
6	2	2	0.02	0	0
7	2	2	0.02	0	0
8	2	2	0.02	0	0
9	2	2	0.02	0	0
10	2	2	0.02	0	0
11	2	2	0.02	0	0
12	2	2	0.02	0	0
13	2	2	0.06	0	0
14	2	2	0.06	0	0
15	2	2	0.06	0	0
16	2	2	0.06	0	0
17	2	2	0.12	0	0
18	2	2	0.12	0	0
19	2	2	0.12	0	0
20	2	2	0.12	0	0
21	2	2	0.12	0	0
22	2	2	0.12	0	0
23	2	2	0.12	0	0
24	2	2	0.12	0	0
25	2	2	0.12	0	0
26	2	2	0.12	0	0
27	2	2	0.12	0	0
28	2	2	0.12	0	0
29	2	2	0.36	0	0
30	2	2	0.36	0	0
31	2	2	0.36	0	0
32	2	2	0.36	0	0
33	3	2	0.15	0	0
34	3	2	0.15	0	0
35	3	2	0.15	0	0
36	3	2	0.15	0	0
37	3	2	0.15	0	0
38	3	2	0.15	0	0
39	3	2	0.15	0	0
40	3	2	0.15	0	0
41	3	2	0.15	0	0
42	3	2	0.15	0	0
43	3	2	0.15	0	0
44	3	2	0.15	0	0

45	3	2	0.45	0	0
46	3	2	0.45	0	0
47	3	2	0.45	0	0
48	3	2	0.45	0	0

INFEXP: Infiltration Exponent

INFILD: Infiltration ratio (maximum to mean)

DEEPFR: Fraction of groundwater to deep aquifer or inactive storage

BASETP: Base flow (from groundwater) Evapotranspiration fraction

AGWETP: Active Groundwater Evapotranspiration fraction

Table 4. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values – Part III

PERLND No.	CEPSC	UZSN	NSUR	INTFW	IRC	LZETP
1	see Table 8	0.45	0.35	2.25	0.60	see Table 9
2	see Table 8	0.35	0.35	2.00	0.50	see Table 9
3	see Table 8	0.25	0.35	1.50	0.45	see Table 9
4	see Table 8	0.20	0.35	1.00	0.40	see Table 9
5	see Table 8	0.40	0.30	2.00	0.50	see Table 9
6	see Table 8	0.30	0.30	1.60	0.45	see Table 9
7	see Table 8	0.20	0.30	1.30	0.40	see Table 9
8	see Table 8	0.15	0.30	0.90	0.35	see Table 9
9	see Table 8	0.35	0.25	2.00	0.50	see Table 9
10	see Table 8	0.30	0.25	1.60	0.45	see Table 9
11	see Table 8	0.23	0.25	1.30	0.40	see Table 9
12	see Table 8	0.20	0.25	0.90	0.35	see Table 9
13	see Table 8	0.35	0.25	1.50	0.40	see Table 9
14	see Table 8	0.30	0.25	1.20	0.35	see Table 9
15	see Table 8	0.23	0.25	0.80	0.30	see Table 9
16	see Table 8	0.20	0.25	0.50	0.30	see Table 9
17	see Table 8	0.45	0.35	2.00	0.60	see Table 9
18	see Table 8	0.35	0.35	1.50	0.50	see Table 9
19	see Table 8	0.25	0.35	1.00	0.45	see Table 9
20	see Table 8	0.20	0.35	0.40	0.40	see Table 9
21	see Table 8	0.40	0.30	1.50	0.50	see Table 9
22	see Table 8	0.30	0.30	1.20	0.45	see Table 9
23	see Table 8	0.20	0.30	0.80	0.40	see Table 9
24	see Table 8	0.15	0.30	0.30	0.35	see Table 9
25	see Table 8	0.35	0.25	1.50	0.50	see Table 9
26	see Table 8	0.30	0.25	1.20	0.45	see Table 9
27	see Table 8	0.23	0.25	0.80	0.40	see Table 9
28	see Table 8	0.20	0.25	0.30	0.35	see Table 9
29	see Table 8	0.35	0.25	1.00	0.40	see Table 9
30	see Table 8	0.30	0.25	0.60	0.35	see Table 9
31	see Table 8	0.23	0.25	0.40	0.30	see Table 9
32	see Table 8	0.20	0.25	0.30	0.30	see Table 9
33	see Table 8	0.35	0.35	0.80	0.60	see Table 9
34	see Table 8	0.30	0.35	0.65	0.50	see Table 9
35	see Table 8	0.25	0.35	0.50	0.45	see Table 9
36	see Table 8	0.20	0.35	0.20	0.40	see Table 9
37	see Table 8	0.30	0.30	0.75	0.50	see Table 9
38	see Table 8	0.25	0.30	0.55	0.45	see Table 9
39	see Table 8	0.20	0.30	0.35	0.40	see Table 9
40	see Table 8	0.15	0.30	0.20	0.35	see Table 9
41	see Table 8	0.30	0.25	0.70	0.50	see Table 9
42	see Table 8	0.25	0.25	0.50	0.45	see Table 9
43	see Table 8	0.20	0.25	0.30	0.40	see Table 9
44	see Table 8	0.15	0.25	0.15	0.35	see Table 9

45	see Table 8	0.25	0.25	0.50	0.40	see Table 9
46	see Table 8	0.23	0.25	0.35	0.35	see Table 9
47	see Table 8	0.20	0.25	0.25	0.30	see Table 9
48	see Table 8	0.15	0.25	0.15	0.30	see Table 9

CEPSC: Interception storage (inches)

UZSN: Upper Zone Storage Nominal (inches)

NSUR: Surface roughness (Manning's n)

INTFW: Interflow index

IRC: Interflow Recession Constant (per day)

LZETP: Lower Zone Evapotranspiration fraction

Table 5. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values – Part IV

PERLND No.	MELEV	BELV	GWDATM	PCW	PGW	UPGW
1	400	0	0	0.35	0.38	0.45
2	400	0	0	0.35	0.38	0.45
3	400	0	0	0.35	0.38	0.45
4	400	0	0	0.35	0.38	0.45
5	400	0	0	0.33	0.35	0.42
6	400	0	0	0.33	0.35	0.42
7	400	0	0	0.33	0.35	0.42
8	400	0	0	0.33	0.35	0.42
9	400	0	0	0.31	0.33	0.40
10	400	0	0	0.31	0.33	0.40
11	400	0	0	0.31	0.33	0.40
12	400	0	0	0.31	0.33	0.40
13	400	0	0	0.30	0.32	0.38
14	400	0	0	0.30	0.32	0.38
15	400	0	0	0.30	0.32	0.38
16	400	0	0	0.30	0.32	0.38
17	400	0	0	0.30	0.32	0.40
18	400	0	0	0.30	0.32	0.40
19	400	0	0	0.30	0.32	0.40
20	400	0	0	0.30	0.32	0.40
21	400	0	0	0.28	0.30	0.37
22	400	0	0	0.28	0.30	0.37
23	400	0	0	0.28	0.30	0.37
24	400	0	0	0.28	0.30	0.37
25	400	0	0	0.26	0.28	0.35
26	400	0	0	0.26	0.28	0.35
27	400	0	0	0.26	0.28	0.35
28	400	0	0	0.26	0.28	0.35
29	400	0	0	0.25	0.27	0.33
30	400	0	0	0.25	0.27	0.33
31	400	0	0	0.25	0.27	0.33
32	400	0	0	0.25	0.27	0.33
33	400	0	0	0.20	0.23	0.28
34	400	0	0	0.20	0.23	0.28
35	400	0	0	0.20	0.23	0.28
36	400	0	0	0.20	0.23	0.28
37	400	0	0	0.18	0.20	0.25
38	400	0	0	0.18	0.20	0.25
39	400	0	0	0.18	0.20	0.25
40	400	0	0	0.18	0.20	0.25
41	400	0	0	0.15	0.17	0.20
42	400	0	0	0.15	0.17	0.20
43	400	0	0	0.15	0.17	0.20
44	400	0	0	0.15	0.17	0.20

45	400	0	0	0.14	0.15	0.18
46	400	0	0	0.14	0.15	0.18
47	400	0	0	0.14	0.15	0.18
48	400	0	0	0.14	0.15	0.18

MELEV: Mean surface elevation of the land segment (feet)

BELV: Base elevation for active groundwater (feet)

GWDATM: Datum for the groundwater elevation (feet)

PCW: Cohesion Water Porosity (fraction)

PGW: Gravitational Water Porosity (fraction)

UPGW: Upper Gravitational Water porosity (fraction)

Table 6. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values – Part V

PERLND No.	STABNO	SRRC	SREXP	IFWSC	DELTA	UELFAC	LELFAC
1	1	0.1	0	4	0.2	4	2.5
2	1	0.1	0	4	0.2	4	2.5
3	1	0.1	0	4	0.2	4	2.5
4	1	0.1	0	4	0.2	4	2.5
5	1	0.1	0	4	0.2	4	2.5
6	1	0.1	0	4	0.2	4	2.5
7	1	0.1	0	4	0.2	4	2.5
8	1	0.1	0	4	0.2	4	2.5
9	1	0.1	0	4	0.2	4	2.5
10	1	0.1	0	4	0.2	4	2.5
11	1	0.1	0	4	0.2	4	2.5
12	1	0.1	0	4	0.2	4	2.5
13	1	0.1	0	4	0.2	4	2.5
14	1	0.1	0	4	0.2	4	2.5
15	1	0.1	0	4	0.2	4	2.5
16	1	0.1	0	4	0.2	4	2.5
17	1	0.1	0	4	0.2	4	2.5
18	1	0.1	0	4	0.2	4	2.5
19	1	0.1	0	4	0.2	4	2.5
20	1	0.1	0	4	0.2	4	2.5
21	1	0.1	0	4	0.2	4	2.5
22	1	0.1	0	4	0.2	4	2.5
23	1	0.1	0	4	0.2	4	2.5
24	1	0.1	0	4	0.2	4	2.5
25	1	0.1	0	4	0.2	4	2.5
26	1	0.1	0	4	0.2	4	2.5
27	1	0.1	0	4	0.2	4	2.5
28	1	0.1	0	4	0.2	4	2.5
29	1	0.1	0	4	0.2	4	2.5
30	1	0.1	0	4	0.2	4	2.5
31	1	0.1	0	4	0.2	4	2.5
32	1	0.1	0	4	0.2	4	2.5
33	1	0.1	0	4	0.2	4	2.5
34	1	0.1	0	4	0.2	4	2.5
35	1	0.1	0	4	0.2	4	2.5
36	1	0.1	0	4	0.2	4	2.5
37	1	0.1	0	4	0.2	4	2.5
38	1	0.1	0	4	0.2	4	2.5
39	1	0.1	0	4	0.2	4	2.5
40	1	0.1	0	4	0.2	4	2.5
41	1	0.1	0	4	0.2	4	2.5
42	1	0.1	0	4	0.2	4	2.5
43	1	0.1	0	4	0.2	4	2.5
44	1	0.1	0	4	0.2	4	2.5

45	1	0.1	0	4	0.2	4	2.5
46	1	0.1	0	4	0.2	4	2.5
47	1	0.1	0	4	0.2	4	2.5
48	1	0.1	0	4	0.2	4	2.5

STABNO: User's number for the FTABLE in the FTABLES block which contains the outflow properties from the surface storage

SRRC: Surface Runoff Recession Constant (per hour)

SREXP: Surface Runoff Exponent

IFWSC: Maximum Interflow Storage Capacity when the groundwater elevation is greater than the upper influence elevation (inches)

DELTA: groundwater tolerance level used to determine transition between regions when high water table conditions are being simulated

UELFAC: multiplier on UZSN which gives the upper zone capacity

LELFAC: multiplier on LZSN which gives the lower zone capacity

The selection of the Table 5 and Table 6 default parameter values is based on limited application of these parameters in San Francisco Bay Area by the staff of Clear Creek Solutions, Inc.

NOTE: The parameter values should be used with caution and only after consultation with the appropriate local municipal permitting agency or guidance provided in Appendix D. Different values should only be selected following detailed local soil analysis, a thorough understanding of the parameters and algorithms, and consultation with the appropriate local municipal permitting agency.

Table 7. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values – Part VI

PERLND No.	CEPS	SURS	UZS	IFWS	LZS	AGWS	GWVS
1	0	0	0.01	0	0.5	0.3	0.01
2	0	0	0.01	0	0.5	0.3	0.01
3	0	0	0.01	0	0.5	0.3	0.01
4	0	0	0.01	0	0.5	0.3	0.01
5	0	0	0.01	0	0.5	0.3	0.01
6	0	0	0.01	0	0.5	0.3	0.01
7	0	0	0.01	0	0.5	0.3	0.01
8	0	0	0.01	0	0.5	0.3	0.01
9	0	0	0.01	0	0.5	0.3	0.01
10	0	0	0.01	0	0.5	0.3	0.01
11	0	0	0.01	0	0.5	0.3	0.01
12	0	0	0.01	0	0.5	0.3	0.01
13	0	0	0.01	0	3.5	1.5	0.10
14	0	0	0.01	0	3.5	1.5	0.10
15	0	0	0.01	0	3.5	1.5	0.10
16	0	0	0.01	0	3.5	1.5	0.10
17	0	0	0.01	0	0.5	0.3	0.01
18	0	0	0.01	0	0.5	0.3	0.01
19	0	0	0.01	0	0.5	0.3	0.01
20	0	0	0.01	0	0.5	0.3	0.01
21	0	0	0.01	0	0.5	0.3	0.01
22	0	0	0.01	0	0.5	0.3	0.01
23	0	0	0.01	0	0.5	0.3	0.01
24	0	0	0.01	0	0.5	0.3	0.01
25	0	0	0.01	0	0.5	0.3	0.01
26	0	0	0.01	0	0.5	0.3	0.01
27	0	0	0.01	0	0.5	0.3	0.01
28	0	0	0.01	0	0.5	0.3	0.01
29	0	0	0.01	0	3.5	1.5	0.10
30	0	0	0.01	0	3.5	1.5	0.10
31	0	0	0.01	0	3.5	1.5	0.10
32	0	0	0.01	0	3.5	1.5	0.10
33	0	0	0.01	0	0.5	0.3	0.01
34	0	0	0.01	0	0.5	0.3	0.01
35	0	0	0.01	0	0.5	0.3	0.01
36	0	0	0.01	0	0.5	0.3	0.01
37	0	0	0.01	0	0.5	0.3	0.01
38	0	0	0.01	0	0.5	0.3	0.01
39	0	0	0.01	0	0.5	0.3	0.01
40	0	0	0.01	0	0.5	0.3	0.01
41	0	0	0.01	0	0.5	0.3	0.01
42	0	0	0.01	0	0.5	0.3	0.01
43	0	0	0.01	0	0.5	0.3	0.01
44	0	0	0.01	0	0.5	0.3	0.01

45	0	0	0.01	0	3.5	1.7	0.10
46	0	0	0.01	0	3.5	1.7	0.10
47	0	0	0.01	0	3.5	1.7	0.10
48	0	0	0.01	0	3.5	1.7	0.10

CEPS: Initial interception storage (inches)

SURS: Initial surface runoff (inches)

UZS: Initial Upper Zone Storage (inches)

IFWS: Initial interflow (inches)

LZS: Initial Lower Zone Storage (inches)

AGWS: Initial Active Groundwater storage (inches)

GWVS: Initial Groundwater Vertical Slope (feet/feet)

Table 8. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values: Monthly Interception Storage (inches)

PERLND No.	JAN	FEB	MAR	APR	MAY	JUN	JUL	AUG	SEP	OCT	NOV	DEC
1	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
2	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
3	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
4	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
5	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
6	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
7	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
8	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
9	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
10	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
11	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
12	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
13	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
14	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
15	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
16	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
17	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
18	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
19	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
20	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
21	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
22	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
23	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
24	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
25	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
26	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
27	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
28	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12

Bay Area Hydrology Model 2023 User Manual – December 2023

29	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
30	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
31	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
32	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
33	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
34	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
35	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
36	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
37	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14
38	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14
39	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14
40	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14
41	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11
42	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11
43	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11
44	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11
45	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
46	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
47	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
48	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11

Table 9. BAHM2023 Alameda/San Mateo/Contra Costa HSPF Pervious Parameter Values: Monthly Lower Zone Evapotranspiration

PERLND No.	JAN	FEB	MAR	APR	MAY	JUN	JUL	AUG	SEP	OCT	NOV	DEC
1	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
2	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
3	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
4	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
5	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
6	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
7	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
8	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
9	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
10	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
11	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
12	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
13	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
14	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
15	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
16	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
17	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
18	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
19	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
20	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
21	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
22	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
23	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
24	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
25	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
26	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
27	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
28	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
29	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50

Bay Area Hydrology Model 2023 User Manual – December 2023

30	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
31	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
32	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
33	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
34	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
35	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
36	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
37	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
38	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
39	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
40	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
41	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.55	0.45	0.40
42	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.55	0.45	0.40
43	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.55	0.45	0.40
44	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.55	0.45	0.40
45	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
46	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
47	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
48	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50

This page has been intentionally left blank.

APPENDIX B: DEFAULT BAHM2023 HSPF PERVIOUS PARAMETER VALUES FOR SANTA CLARA COUNTY

The default BAHM2023 HSPF pervious parameter values are found in BAHM2023 file defaultpers.uci. These pervious parameter values have not changed from the original BAHM values.

The default BAHM2023 HSPF pervious parameter values for Santa Clara County are based on the HSPF calibration of Ross Creek. The default BAHM2023 HSPF pervious parameter values for Alameda and San Mateo counties are listed in Appendix A.

The HSPF calibrations of Ross Creek and Thompson Creek are documented in the report: Clear Creek Solutions. 2007. Hydrologic Modeling of the Ross Creek and Thompson Creek Watersheds with the U.S. EPA Hydrologic Simulation Program – FORTRAN (HSPF). Prepared for Santa Clara Valley Urban Runoff Pollution Prevention Program.

Any changes in the default BAHM2023 HSPF pervious and impervious parameter values require approval by the local municipal permitting agency, unless covered by additional guidance in Appendix D.

HSPF parameter documentation is found in the document:
Bicknell, B.R., J.C. Imhoff, J.L. Kittle Jr, T.H. Jobes, and A.S. Donigian Jr. 2001. Hydrological Simulation Program – Fortran, User's Manual for Version 12. AQUA TERRA Consultants. Mountain View, CA.

Table 1. BAHM2023 Santa Clara Pervious Land Types

PERLND No.	Soil	Vegetation/Surface	Slope
1	A	Forest	Flat(0-5%)
2	A	Forest	Moderate(5-10%)
3	A	Forest	Steep(10-20%)
4	A	Forest	Very Steep(>20%)
5	A	Shrub	Flat(0-5%)
6	A	Shrub	Moderate(5-10%)
7	A	Shrub	Steep(10-20%)
8	A	Shrub	Very Steep(>20%)
9	A	Grass	Flat(0-5%)
10	A	Grass	Moderate(5-10%)
11	A	Grass	Steep(10-20%)
12	A	Grass	Very Steep(>20%)
13	A	Urban	Flat(0-5%)
14	A	Urban	Moderate(5-10%)
15	A	Urban	Steep(10-20%)
16	A	Urban	Very Steep(>20%)
17	B	Forest	Flat(0-5%)
18	B	Forest	Moderate(5-10%)
19	B	Forest	Steep(10-20%)
20	B	Forest	Very Steep(>20%)
21	B	Shrub	Flat(0-5%)
22	B	Shrub	Moderate(5-10%)
23	B	Shrub	Steep(10-20%)
24	B	Shrub	Very Steep(>20%)
25	B	Grass	Flat(0-5%)
26	B	Grass	Moderate(5-10%)
27	B	Grass	Steep(10-20%)
28	B	Grass	Very Steep(>20%)
29	B	Urban	Flat(0-5%)
30	B	Urban	Moderate(5-10%)
31	B	Urban	Steep(10-20%)
32	B	Urban	Very Steep(>20%)
33	C/D	Forest	Flat(0-5%)
34	C/D	Forest	Moderate(5-10%)
35	C/D	Forest	Steep(10-20%)
36	C/D	Forest	Very Steep(>20%)
37	C/D	Shrub	Flat(0-5%)
38	C/D	Shrub	Moderate(5-10%)
39	C/D	Shrub	Steep(10-20%)
40	C/D	Shrub	Very Steep(>20%)
41	C/D	Grass	Flat(0-5%)
42	C/D	Grass	Moderate(5-10%)
43	C/D	Grass	Steep(10-20%)
44	C/D	Grass	Very Steep(>20%)
45	C/D	Urban	Flat(0-5%)

46	C/D	Urban	Moderate(5-10%)
47	C/D	Urban	Steep(10-20%)
48	C/D	Urban	Very Steep(>20%)

Table 2. BAHM2023 Santa Clara HSPF Pervious Parameter Values – Part I

PERLND No.	LZSN	INFILT	LSUR	SLSUR	KVARY	AGWRC
1	5.2	0.100	400	0.05	0.8	0.985
2	4.8	0.075	350	0.10	0.8	0.985
3	4.5	0.055	300	0.15	0.8	0.985
4	4.2	0.045	200	0.25	0.8	0.985
5	5.2	0.090	400	0.05	0.8	0.955
6	4.8	0.070	350	0.10	0.8	0.955
7	4.5	0.045	300	0.15	0.8	0.955
8	4.2	0.040	200	0.25	0.8	0.955
9	5.2	0.090	400	0.05	0.8	0.955
10	4.8	0.070	350	0.10	0.8	0.955
11	4.5	0.045	300	0.15	0.8	0.955
12	4.2	0.040	200	0.25	0.8	0.955
13	5.0	0.060	400	0.05	1.2	0.997
14	4.6	0.050	350	0.10	1.2	0.997
15	4.2	0.040	300	0.15	1.2	0.997
16	3.8	0.030	200	0.25	1.2	0.997
17	5.0	0.080	400	0.05	1.2	0.980
18	4.7	0.060	350	0.10	1.2	0.980
19	4.4	0.045	300	0.15	1.2	0.980
20	4.1	0.035	200	0.25	1.2	0.980
21	5.0	0.070	400	0.05	1.2	0.950
22	4.7	0.055	350	0.10	1.2	0.950
23	4.4	0.040	300	0.15	1.2	0.950
24	4.1	0.030	200	0.25	1.2	0.950
25	5.0	0.070	400	0.05	1.2	0.950
26	4.7	0.055	350	0.10	1.2	0.950
27	4.4	0.040	300	0.15	1.2	0.950
28	4.1	0.030	200	0.25	1.2	0.950
29	4.8	0.050	400	0.05	1.8	0.995
30	4.4	0.040	350	0.10	1.8	0.995
31	4.0	0.030	300	0.15	1.8	0.995
32	3.6	0.025	200	0.25	1.8	0.995
33	4.8	0.050	400	0.05	2.0	0.980
34	4.5	0.045	350	0.10	2.0	0.980
35	4.2	0.035	300	0.15	2.0	0.980
36	4.0	0.030	200	0.25	2.0	0.980
37	4.8	0.045	400	0.05	2.0	0.950
38	4.5	0.040	350	0.10	2.0	0.950
39	4.2	0.030	300	0.15	2.0	0.950
40	4.0	0.025	200	0.25	2.0	0.950
41	4.8	0.045	400	0.05	2.0	0.950
42	4.5	0.040	350	0.10	2.0	0.950
43	4.2	0.030	300	0.15	2.0	0.950
44	4.0	0.025	200	0.25	2.0	0.950
45	4.6	0.040	400	0.05	3.0	0.995

46	4.2	0.030	350	0.10	3.0	0.995
47	3.8	0.022	300	0.15	3.0	0.995
48	3.5	0.020	200	0.25	3.0	0.995

LZSN: Lower Zone Storage Nominal (inches)

INFILT: Infiltration (inches per hour)

LSUR: Length of surface flow path (feet)

SLSUR: Slope of surface flow path (feet/feet)

KVARY: Variable groundwater recession

AGWRC: Active Groundwater Recession Constant (per day)

Table 3. BAHM2023 Santa Clara HSPF Pervious Parameter Values – Part II

PERLND No.	INFEXP	INFILD	DEEPPFR	BASETP	AGWETP
1	2	2	0.5	0	0
2	2	2	0.5	0	0
3	2	2	0.5	0	0
4	2	2	0.5	0	0
5	2	2	0.5	0	0
6	2	2	0.5	0	0
7	2	2	0.5	0	0
8	2	2	0.5	0	0
9	2	2	0.5	0	0
10	2	2	0.5	0	0
11	2	2	0.5	0	0
12	2	2	0.5	0	0
13	2	2	0.5	0	0
14	2	2	0.5	0	0
15	2	2	0.5	0	0
16	2	2	0.5	0	0
17	2	2	0.5	0	0
18	2	2	0.5	0	0
19	2	2	0.5	0	0
20	2	2	0.5	0	0
21	2	2	0.5	0	0
22	2	2	0.5	0	0
23	2	2	0.5	0	0
24	2	2	0.5	0	0
25	2	2	0.5	0	0
26	2	2	0.5	0	0
27	2	2	0.5	0	0
28	2	2	0.5	0	0
29	2	2	0.5	0	0
30	2	2	0.5	0	0
31	2	2	0.5	0	0
32	2	2	0.5	0	0
33	3	2	0.5	0	0
34	3	2	0.5	0	0
35	3	2	0.5	0	0
36	3	2	0.5	0	0
37	3	2	0.5	0	0
38	3	2	0.5	0	0
39	3	2	0.5	0	0
40	3	2	0.5	0	0
41	3	2	0.5	0	0
42	3	2	0.5	0	0
43	3	2	0.5	0	0
44	3	2	0.5	0	0
45	3	2	0.5	0	0

46	3	2	0.5	0	0
47	3	2	0.5	0	0
48	3	2	0.5	0	0

INFEXP: Infiltration Exponent

INFILD: Infiltration ratio (maximum to mean)

DEEPFR: Fraction of groundwater to deep aquifer or inactive storage

BASETP: Base flow (from groundwater) Evapotranspiration fraction

AGWETP: Active Groundwater Evapotranspiration fraction

Table 4. BAHM2023 Santa Clara HSPF Pervious Parameter Values – Part III

PERLND No.	CEPSC	UZSN	NSUR	INTFW	IRC	LZETP
1	see Table 8	0.50	0.35	1.00	0.80	see Table 9
2	see Table 8	0.40	0.35	0.95	0.50	see Table 9
3	see Table 8	0.30	0.35	0.90	0.45	see Table 9
4	see Table 8	0.25	0.35	0.80	0.40	see Table 9
5	see Table 8	0.45	0.30	0.95	0.70	see Table 9
6	see Table 8	0.35	0.30	0.90	0.45	see Table 9
7	see Table 8	0.25	0.30	0.80	0.40	see Table 9
8	see Table 8	0.20	0.30	0.60	0.35	see Table 9
9	see Table 8	0.40	0.25	0.95	0.70	see Table 9
10	see Table 8	0.35	0.25	0.90	0.45	see Table 9
11	see Table 8	0.28	0.25	0.80	0.40	see Table 9
12	see Table 8	0.25	0.25	0.60	0.35	see Table 9
13	see Table 8	0.40	0.25	0.90	0.40	see Table 9
14	see Table 8	0.35	0.25	0.80	0.35	see Table 9
15	see Table 8	0.28	0.25	0.70	0.30	see Table 9
16	see Table 8	0.25	0.25	0.60	0.30	see Table 9
17	see Table 8	0.50	0.35	1.00	0.80	see Table 9
18	see Table 8	0.40	0.35	0.95	0.50	see Table 9
19	see Table 8	0.30	0.35	0.90	0.45	see Table 9
20	see Table 8	0.25	0.35	0.80	0.40	see Table 9
21	see Table 8	0.45	0.30	0.95	0.70	see Table 9
22	see Table 8	0.35	0.30	0.90	0.45	see Table 9
23	see Table 8	0.25	0.30	0.80	0.40	see Table 9
24	see Table 8	0.20	0.30	0.60	0.35	see Table 9
25	see Table 8	0.40	0.25	0.95	0.70	see Table 9
26	see Table 8	0.35	0.25	0.90	0.45	see Table 9
27	see Table 8	0.28	0.25	0.80	0.40	see Table 9
28	see Table 8	0.25	0.25	0.60	0.35	see Table 9
29	see Table 8	0.40	0.25	0.90	0.40	see Table 9
30	see Table 8	0.35	0.25	0.80	0.35	see Table 9
31	see Table 8	0.28	0.25	0.70	0.30	see Table 9
32	see Table 8	0.25	0.25	0.60	0.30	see Table 9
33	see Table 8	0.40	0.35	1.00	0.80	see Table 9
34	see Table 8	0.35	0.35	0.95	0.50	see Table 9
35	see Table 8	0.25	0.35	0.90	0.45	see Table 9
36	see Table 8	0.20	0.35	0.80	0.40	see Table 9
37	see Table 8	0.35	0.30	0.95	0.70	see Table 9
38	see Table 8	0.30	0.30	0.90	0.45	see Table 9
39	see Table 8	0.25	0.30	0.80	0.40	see Table 9
40	see Table 8	0.20	0.30	0.60	0.35	see Table 9
41	see Table 8	0.35	0.25	0.95	0.70	see Table 9
42	see Table 8	0.30	0.25	0.90	0.45	see Table 9
43	see Table 8	0.25	0.25	0.80	0.40	see Table 9
44	see Table 8	0.20	0.25	0.60	0.35	see Table 9
45	see Table 8	0.30	0.25	0.80	0.40	see Table 9

46	see Table 8	0.28	0.25	0.70	0.35	see Table 9
47	see Table 8	0.25	0.25	0.50	0.30	see Table 9
48	see Table 8	0.20	0.25	0.35	0.30	see Table 9

CEPSC: Interception storage (inches)

UZSN: Upper Zone Storage Nominal (inches)

NSUR: Surface roughness (Manning's n)

INTFW: Interflow index

IRC: Interflow Recession Constant (per day)

LZETP: Lower Zone Evapotranspiration fraction

Table 5. BAHM2023 Santa Clara HSPF Pervious Parameter Values – Part IV

PERLND No.	MELEV	BELV	GWDATM	PCW	PGW	UPGW
1	400	0	0	0.35	0.38	0.45
2	400	0	0	0.35	0.38	0.45
3	400	0	0	0.35	0.38	0.45
4	400	0	0	0.35	0.38	0.45
5	400	0	0	0.33	0.35	0.42
6	400	0	0	0.33	0.35	0.42
7	400	0	0	0.33	0.35	0.42
8	400	0	0	0.33	0.35	0.42
9	400	0	0	0.31	0.33	0.40
10	400	0	0	0.31	0.33	0.40
11	400	0	0	0.31	0.33	0.40
12	400	0	0	0.31	0.33	0.40
13	400	0	0	0.30	0.32	0.38
14	400	0	0	0.30	0.32	0.38
15	400	0	0	0.30	0.32	0.38
16	400	0	0	0.30	0.32	0.38
17	400	0	0	0.30	0.32	0.40
18	400	0	0	0.30	0.32	0.40
19	400	0	0	0.30	0.32	0.40
20	400	0	0	0.30	0.32	0.40
21	400	0	0	0.28	0.30	0.37
22	400	0	0	0.28	0.30	0.37
23	400	0	0	0.28	0.30	0.37
24	400	0	0	0.28	0.30	0.37
25	400	0	0	0.26	0.28	0.35
26	400	0	0	0.26	0.28	0.35
27	400	0	0	0.26	0.28	0.35
28	400	0	0	0.26	0.28	0.35
29	400	0	0	0.25	0.27	0.33
30	400	0	0	0.25	0.27	0.33
31	400	0	0	0.25	0.27	0.33
32	400	0	0	0.25	0.27	0.33
33	400	0	0	0.20	0.23	0.28
34	400	0	0	0.20	0.23	0.28
35	400	0	0	0.20	0.23	0.28
36	400	0	0	0.20	0.23	0.28
37	400	0	0	0.18	0.20	0.25
38	400	0	0	0.18	0.20	0.25
39	400	0	0	0.18	0.20	0.25
40	400	0	0	0.18	0.20	0.25
41	400	0	0	0.15	0.17	0.20
42	400	0	0	0.15	0.17	0.20
43	400	0	0	0.15	0.17	0.20
44	400	0	0	0.15	0.17	0.20
45	400	0	0	0.14	0.15	0.18

46	400	0	0	0.14	0.15	0.18
47	400	0	0	0.14	0.15	0.18
48	400	0	0	0.14	0.15	0.18

MELEV: Mean surface elevation of the land segment (feet)

BELV: Base elevation for active groundwater (feet)

GWDATM: Datum for the groundwater elevation (feet)

PCW: Cohesion Water Porosity (fraction)

PGW: Gravitational Water Porosity (fraction)

UPGW: Upper Gravitational Water porosity (fraction)

Table 6. BAHM2023 Santa Clara HSPF Pervious Parameter Values – Part V

PERLND No.	STABNO	SRRRC	SREXP	IFWSC	DELTA	UELFAC	LELFAC
1	1	0.1	0	4	0.2	4	2.5
2	1	0.1	0	4	0.2	4	2.5
3	1	0.1	0	4	0.2	4	2.5
4	1	0.1	0	4	0.2	4	2.5
5	1	0.1	0	4	0.2	4	2.5
6	1	0.1	0	4	0.2	4	2.5
7	1	0.1	0	4	0.2	4	2.5
8	1	0.1	0	4	0.2	4	2.5
9	1	0.1	0	4	0.2	4	2.5
10	1	0.1	0	4	0.2	4	2.5
11	1	0.1	0	4	0.2	4	2.5
12	1	0.1	0	4	0.2	4	2.5
13	1	0.1	0	4	0.2	4	2.5
14	1	0.1	0	4	0.2	4	2.5
15	1	0.1	0	4	0.2	4	2.5
16	1	0.1	0	4	0.2	4	2.5
17	1	0.1	0	4	0.2	4	2.5
18	1	0.1	0	4	0.2	4	2.5
19	1	0.1	0	4	0.2	4	2.5
20	1	0.1	0	4	0.2	4	2.5
21	1	0.1	0	4	0.2	4	2.5
22	1	0.1	0	4	0.2	4	2.5
23	1	0.1	0	4	0.2	4	2.5
24	1	0.1	0	4	0.2	4	2.5
25	1	0.1	0	4	0.2	4	2.5
26	1	0.1	0	4	0.2	4	2.5
27	1	0.1	0	4	0.2	4	2.5
28	1	0.1	0	4	0.2	4	2.5
29	1	0.1	0	4	0.2	4	2.5
30	1	0.1	0	4	0.2	4	2.5
31	1	0.1	0	4	0.2	4	2.5
32	1	0.1	0	4	0.2	4	2.5
33	1	0.1	0	4	0.2	4	2.5
34	1	0.1	0	4	0.2	4	2.5
35	1	0.1	0	4	0.2	4	2.5
36	1	0.1	0	4	0.2	4	2.5
37	1	0.1	0	4	0.2	4	2.5
38	1	0.1	0	4	0.2	4	2.5
39	1	0.1	0	4	0.2	4	2.5
40	1	0.1	0	4	0.2	4	2.5
41	1	0.1	0	4	0.2	4	2.5
42	1	0.1	0	4	0.2	4	2.5
43	1	0.1	0	4	0.2	4	2.5
44	1	0.1	0	4	0.2	4	2.5
45	1	0.1	0	4	0.2	4	2.5

46	1	0.1	0	4	0.2	4	2.5
47	1	0.1	0	4	0.2	4	2.5
48	1	0.1	0	4	0.2	4	2.5

STABNO: User's number for the FTABLE in the FTABLES block which contains the outflow properties from the surface storage

SRRC: Surface Runoff Recession Constant (per hour)

SREXP: Surface Runoff Exponent

IFWSC: Maximum Interflow Storage Capacity when the groundwater elevation is greater than the upper influence elevation (inches)

DELTA: groundwater tolerance level used to determine transition between regions when high water table conditions are being simulated

UELFAC: multiplier on UZSN which gives the upper zone capacity

LELFAC: multiplier on LZSN which gives the lower zone capacity

The selection of the Table 5 and Table 6 default parameter values is based on limited application of these parameters in San Francisco Bay Area by the staff of Clear Creek Solutions, Inc.

NOTE: The parameter values should be used with caution and only after consultation with the appropriate local municipal permitting agency or guidance in Appendix D. Different values should only be selected following detailed local soil analysis, a thorough understanding of the parameters and algorithms, and consultation with the appropriate local municipal permitting agency.

Table 7. BAHM2023 Santa Clara HSPF Pervious Parameter Values – Part VI

PERLND No.	CEPS	SURS	UZS	IFWS	LZS	AGWS	GWVS
1	0	0	0.01	0	0.5	0.3	0.01
2	0	0	0.01	0	0.5	0.3	0.01
3	0	0	0.01	0	0.5	0.3	0.01
4	0	0	0.01	0	0.5	0.3	0.01
5	0	0	0.01	0	0.5	0.3	0.01
6	0	0	0.01	0	0.5	0.3	0.01
7	0	0	0.01	0	0.5	0.3	0.01
8	0	0	0.01	0	0.5	0.3	0.01
9	0	0	0.01	0	0.5	0.3	0.01
10	0	0	0.01	0	0.5	0.3	0.01
11	0	0	0.01	0	0.5	0.3	0.01
12	0	0	0.01	0	0.5	0.3	0.01
13	0	0	0.01	0	3.5	1.5	0.10
14	0	0	0.01	0	3.5	1.5	0.10
15	0	0	0.01	0	3.5	1.5	0.10
16	0	0	0.01	0	3.5	1.5	0.10
17	0	0	0.01	0	0.5	0.3	0.01
18	0	0	0.01	0	0.5	0.3	0.01
19	0	0	0.01	0	0.5	0.3	0.01
20	0	0	0.01	0	0.5	0.3	0.01
21	0	0	0.01	0	0.5	0.3	0.01
22	0	0	0.01	0	0.5	0.3	0.01
23	0	0	0.01	0	0.5	0.3	0.01
24	0	0	0.01	0	0.5	0.3	0.01
25	0	0	0.01	0	0.5	0.3	0.01
26	0	0	0.01	0	0.5	0.3	0.01
27	0	0	0.01	0	0.5	0.3	0.01
28	0	0	0.01	0	0.5	0.3	0.01
29	0	0	0.01	0	3.5	1.5	0.10
30	0	0	0.01	0	3.5	1.5	0.10
31	0	0	0.01	0	3.5	1.5	0.10
32	0	0	0.01	0	3.5	1.5	0.10
33	0	0	0.01	0	0.5	0.3	0.01
34	0	0	0.01	0	0.5	0.3	0.01
35	0	0	0.01	0	0.5	0.3	0.01
36	0	0	0.01	0	0.5	0.3	0.01
37	0	0	0.01	0	0.5	0.3	0.01
38	0	0	0.01	0	0.5	0.3	0.01
39	0	0	0.01	0	0.5	0.3	0.01
40	0	0	0.01	0	0.5	0.3	0.01
41	0	0	0.01	0	0.5	0.3	0.01
42	0	0	0.01	0	0.5	0.3	0.01
43	0	0	0.01	0	0.5	0.3	0.01
44	0	0	0.01	0	0.5	0.3	0.01
45	0	0	0.01	0	3.5	1.7	0.10

46	0	0	0.01	0	3.5	1.7	0.10
47	0	0	0.01	0	3.5	1.7	0.10
48	0	0	0.01	0	3.5	1.7	0.10

CEPS: Initial interception storage (inches)

SURS: Initial surface runoff (inches)

UZS: Initial Upper Zone Storage (inches)

IFWS: Initial interflow (inches)

LZS: Initial Lower Zone Storage (inches)

AGWS: Initial Active Groundwater storage (inches)

GWVS: Initial Groundwater Vertical Slope (feet/feet)

Table 8. BAHM2023 Santa Clara HSPF Pervious Parameter Values: Monthly Interception Storage (inches)

PERLND No.	JAN	FEB	MAR	APR	MAY	JUN	JUL	AUG	SEP	OCT	NOV	DEC
1	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
2	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
3	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
4	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
5	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
6	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
7	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
8	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
9	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
10	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
11	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
12	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
13	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
14	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
15	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
16	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
17	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
18	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
19	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
20	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18
21	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
22	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
23	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
24	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
25	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
26	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
27	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
28	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12

Bay Area Hydrology Model 2023 User Manual – December 2023

29	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	
30	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	
31	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	
32	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	
33	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18	
34	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18	
35	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18	
36	0.15	0.15	0.15	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.20	0.18	
37	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
38	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
39	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
40	0.13	0.13	0.13	0.14	0.15	0.15	0.15	0.15	0.15	0.15	0.15	0.14	0.13
41	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
42	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
43	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
44	0.12	0.12	0.12	0.11	0.10	0.10	0.10	0.10	0.10	0.10	0.10	0.11	0.12
45	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
46	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
47	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11
48	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11	0.11

Table 9. BAHM2023 HSPF Pervious Parameter Values: Monthly Lower Zone Evapotranspiration

PERLND No.	JAN	FEB	MAR	APR	MAY	JUN	JUL	AUG	SEP	OCT	NOV	DEC
1	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
2	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
3	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
4	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
5	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
6	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
7	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
8	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
9	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
10	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
11	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
12	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
13	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
14	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
15	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
16	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
17	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
18	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
19	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
20	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
21	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
22	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
23	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
24	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
25	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
26	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
27	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
28	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
29	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50

30	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
31	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
32	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
33	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
34	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
35	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
36	0.60	0.60	0.60	0.70	0.75	0.75	0.75	0.75	0.75	0.75	0.65	0.60
37	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
38	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
39	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
40	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
41	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
42	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
43	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
44	0.40	0.40	0.40	0.45	0.50	0.55	0.55	0.55	0.55	0.55	0.45	0.40
45	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
46	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
47	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50
48	0.50	0.50	0.50	0.60	0.65	0.65	0.65	0.65	0.65	0.65	0.55	0.50

This page has been intentionally left blank.

APPENDIX C: DEFAULT BAHM2023 HSPF IMPERVIOUS PARAMETER VALUES FOR ALAMEDA, SANTA CLARA, SAN MATEO, AND CONTRA COSTA COUNTIES

The default BAHM2023 HSPF impervious parameter values are found in BAHM2023 file defaultpers.uci. These impervious parameter values have not changed from the original BAHM values.

The default BAHM2023 HSPF impervious parameter values are based on HSPF calibrations of Castro Valley Creek, Alameda Creek, and Ross Creek.

HSPF calibrations of Castro Valley Creek and Alameda Creek are documented in the report:

AQUA TERRA Consultants. 2006. Hydrologic Modeling of the Castro Valley Creek and Alameda Creek Watersheds with the U.S. EPA Hydrologic Simulation Program – FORTRAN (HSPF). Prepared for Alameda Countywide Clean Water Program. January 20, 2006.

The HSPF calibrations of Ross Creek and Thompson Creek are documented in the report: Clear Creek Solutions. 2007. Hydrologic Modeling of the Ross Creek and Thompson Creek Watersheds with the U.S. EPA Hydrologic Simulation Program – FORTRAN (HSPF). Prepared for Santa Clara Valley Urban Runoff Pollution Prevention Program.

Any changes in the default BAHM2023 HSPF pervious and impervious parameter values require approval by the local municipal permitting agency, unless covered by additional guidance in Appendix D.

HSPF parameter documentation is found in the document:

Bicknell, B.R., J.C. Imhoff, J.L. Kittle Jr, T.H. Jobes, and A.S. Donigian Jr. 2001. Hydrological Simulation Program – Fortran, User's Manual for Version 12. AQUA TERRA Consultants. Mountain View, CA.

Table 1. BAHM2023 Impervious Land Types

IMPLND No.	Surface	Slope
1	Roads	Flat(0-5%)
2	Roads	Moderate(5-10%)
3	Roads	Steep(10-20%)
4	Roads	Very Steep(>20%)
5	Roof Area	All
6	Driveways	Flat(0-5%)
7	Driveways	Moderate(5-10%)
8	Driveways	Steep(10-20%)
9	Driveways	Very Steep(>20%)
10	Sidewalks	Flat(0-5%)
11	Sidewalks	Moderate(5-10%)
12	Sidewalks	Steep(10-20%)
13	Sidewalks	Very Steep(>20%)
14	Parking	Flat(0-5%)
15	Parking	Moderate(5-10%)
16	Parking	Steep(10-20%)
17	Parking	Very Steep(>20%)

Table 2. BAHM2023 HSPF Impervious Parameter Values – Part I

IMPLND No.	LSUR	SLSUR	NSUR	RETSC
1	100	0.05	0.1	0.10
2	100	0.10	0.1	0.09
3	100	0.15	0.1	0.08
4	100	0.25	0.1	0.06
5	100	0.05	0.1	0.10
6	100	0.05	0.1	0.10
7	100	0.10	0.1	0.09
8	100	0.15	0.1	0.08
9	100	0.25	0.1	0.06
10	100	0.05	0.1	0.10
11	100	0.10	0.1	0.09
12	100	0.15	0.1	0.08
13	100	0.25	0.1	0.06
14	100	0.05	0.1	0.10
15	100	0.10	0.1	0.09
16	100	0.15	0.1	0.08
17	100	0.25	0.1	0.06

LSUR: Length of surface flow path (feet) for impervious area

SLSUR: Slope of surface flow path (feet/feet) for impervious area

NSUR: Surface roughness (Manning’s n) for impervious area

RETSC: Surface retention storage (inches) for impervious area

Table 3. BAHM2023 HSPF Impervious Parameter Values – Part II

IMPLND No.	RETS	SURS
1	0.00	0.00
2	0.00	0.00
3	0.00	0.00
4	0.00	0.00
5	0.00	0.00
6	0.00	0.00
7	0.00	0.00
8	0.00	0.00
9	0.00	0.00
10	0.00	0.00
11	0.00	0.00
12	0.00	0.00
13	0.00	0.00
14	0.00	0.00
15	0.00	0.00
16	0.00	0.00
17	0.00	0.00
18	0.00	0.00

RETSC: Initial surface retention storage (inches) for impervious area

SURS: Initial surface runoff (inches) for impervious area

APPENDIX D: ADDITIONAL GUIDANCE FOR USING BAHM2023

Scope and Purpose

This appendix includes guidance and background information that are not incorporated into the BAHM2023 software, but which the user needs to know in order to use BAHM2023 for designing projects in the participating jurisdictions. The first section provides a comparison of the terminology used by the BAHM2023 software and user manual with that used in guidance documents developed by Bay Area countywide stormwater programs for compliance with stormwater permit requirements.

The three other topic areas in this appendix are flagged in the main user manual text by specially formatted notes under the BAHM2023 elements or software features to which they are related:

Appendix D Topic	Relevant Sections in User Manual
Infiltration Reduction Factor	Infiltration, page 123; applicable when specifying characteristics of a facility (pond, vault, tank, some LID elements) if “yes” is selected as the Infiltration option.
Flow Duration Outlet Structures (includes sizing of low-flow orifice and alternative configurations)	Outlet Structure Configurations, pages 115-122; applicable when specifying characteristics of a flow duration facility.
Drawdown (drain) time for flow duration facilities	Drawdown (Analysis screen), page 139.

Additional guidance and references are also discussed at the end of this appendix.

The sponsoring stormwater programs may revise and expand this section as time and resources allow. Check the BAHM2023 website at <https://www.clearcreeksolutions.info/bahm-download-page> for the most recent updates.

Terminology and Countywide Specific Guidance

BAHM2023 incorporates terminology from the original BAHM, WWHM, and HSPF models describing site features, model elements, LID treatment facilities, and hydromodification control facilities. The following table provides a comparison between the BAHM2023 terminology, and the terms commonly used in Bay Area countywide stormwater program guidance documents for compliance with stormwater permit requirements. The table also includes notes regarding limitations on the use of certain control facilities in certain counties as described in the countywide guidance. The user should refer to the countywide guidance documents for more specific guidance.

**Cross Reference Table:
BAHM Terminology and Bay Area Countywide Program Guidance**

BAHM Term	Definition	Countywide Program Guidance Term	Additional Countywide Program Guidance
Basin	A land use basin element used to represent the project drainage area or the area that drains to a treatment measure or hydromodification management (HM) facility	<ul style="list-style-type: none"> • Total project area draining to a point of compliance; or • Drainage Management Area (DMA) – if referring to the basin element draining to a treatment measure or HM facility 	
Pond	Surface storage facility (either with a trapezoidal or irregularly shaped top edge) with an outlet structure to control outflow to meet HM standards; can allow infiltration	<ul style="list-style-type: none"> • Detention basin • Self-retaining area (represented by shallow pond) 	<ul style="list-style-type: none"> • Not an LID treatment option (except when used to represent a self-retaining area) • Not an HM option allowed by CCCWP
Vault	Below-ground, rectangular storage facility with an outlet structure to control outflow to meet HM standards; can allow infiltration	Storage vault	
Tank	Below-ground storage facility, represented by a cylinder placed on its side (either circular or an arched half-cylinder with open bottom) with an outlet structure to control outflow to meet HM standards; can allow infiltration	<ul style="list-style-type: none"> • Large diameter pipe (circular tank) • Subsurface infiltration system (arched half-cylinder) 	
BMP	Best management practice for treatment and/or HM control	<ul style="list-style-type: none"> • IMP (CCCWP) • Stormwater Treatment or HM Control Measure (SCVURPPP) 	
Bioretention	Landscaped treatment system with sloped sides using biotreatment soil underlain by gravel, with optional underdrain, allowing infiltration	Bioretention	Select “BAHM5” as the top layer to represent approved Bay Area biotreatment soil mix

BAHM Term	Definition	Countywide Program Guidance Term	Additional Countywide Program Guidance
In-Ground Infiltration Planter	Bioretention facility with vertical sides and an open bottom allowing infiltration to native soil and optional underdrain	<ul style="list-style-type: none"> • Bioretention • Bioinfiltration 	Select “BAHM5” as the top layer to represent approved Bay Area bio-treatment soil mix; CCCWP requires under-drains
Flow-Through Planter	Bioretention facility with vertical sides, solid bottom, and underdrain; no infiltration allowed	<ul style="list-style-type: none"> • Biotreatment • Flow-through planter 	Select “BAHM5” as the top layer to represent approved Bay Area bio-treatment soil mix
Permeable Pavement	Surface layer of porous asphalt, porous concrete, concrete pavers, or grid pavement underlain by one or two subgrade layers of gravel or sand	Permeable, pervious, or porous pavement	
Gravel Trench	Gravel-filled trench allowing infiltration into native soil (may include underdrain)	Infiltration trench with underdrain	
Infiltration Trench	A gravel-filled trench with no underdrain (all water must infiltrate into native soil)	Infiltration trench with no underdrain	Underdrain generally recommended (i.e., use gravel trench)
Dry well	In-ground Infiltration Planter, Infiltration Trench or Gravel Trench with no underdrain (all water must infiltrate into native soil)	Dry well	
Infiltration Basin	Trapezoidal “pond” that can infiltrate stored water into native soil at a specified rate	Infiltration basin	Not an HM option allowed by CCCWP
Dispersion	Method of allowing an impervious “lateral” basin to flow onto a pervious “lateral” basin which infiltrates some of the runoff before routing the rest to an HM control facility	One way of representing a self-retaining area	
Green Roof	Roof area covered with vegetation and soil media (drainage through media is represented as “groundwater” that contributes to the total runoff)	Green roof	

Infiltration Reduction Factor

The Western Washington Hydrology Model included this factor to reflect the requirement in the *Stormwater Management Manual for Western Washington* (SMMWW), to incorporate a Correction Factor (CF) to determine long-term infiltration rates; the inverse of the CF is the Infiltration Reduction Factor in BAHM. The SMMWW gives three methods for determining CF: 1) a table providing empirical correlations between long-term infiltration rates and USDA Soil Textural Classification; 2) ASTM gradation testing at full-scale infiltration facilities; or 3) In-situ infiltration tests, preferably using a Pilot Infiltration Test specified in an appendix of the SMMWW.

Application of a CF or safety factor attempts to account for clogging and the reduction in infiltration over time, which might apply to the bottom of a flow duration pond or infiltration facility. However, a safety factor is also used to account for uncertainties in the available estimate of in-situ infiltration rates. The SMMWW notes that its suggested CF values, which range from 2 to 4, “represent an average degree of long-term facility maintenance, TSS reduction through pretreatment, and site variability in the subsurface conditions”, and that increases or decreases to these factors should be considered for unusual situations.

Suggested safety factors in other texts and guidance generally range from 1 to 4. While a safety factor is recommended, for the reasons described above, designers should not be overly conservative in selecting a very high safety factor, since this might lead to over-controlled (lower) post-project flows and an increased risk of causing impacts from deposition or sedimentation in the receiving channels. In the absence of other guidance, it is suggested that the selected BAHM2023 Infiltration Reduction Factor (the inverse of the safety factor) be between 0.25 and 0.5.

Note: Bay Area countywide stormwater programs may specify the required infiltration reduction factor and/or restrict the use of infiltration for treatment purposes in certain conditions; designers should refer to the “C.3” guidance on treatment measure design for the applicable jurisdiction (see weblinks under Additional Resources below).

Flow Duration Outlet Structures – Practical Design Considerations

Low-flow Orifice Sizing

The diameter of the low-flow (bottom) orifice is an important design parameter for flow duration facilities, since flows discharged through this outlet should be at or below the project threshold for controlled flows (Q_{cp}). However, maintenance and/or other practical considerations may dictate a practical limit to how small this orifice may be, which may be larger than the optimal theoretical diameter determined by Auto Pond (or Auto Vault or Auto Tank). As an example, the SWMMWW specifies a minimum orifice diameter of 0.5 inches, for flow restrictor assemblies that are within protective enclosures that screen out large particles and also have 1-2 ft of sump below the orifice to allow for some sediment accumulation.

While the user can manually set a minimum size for the low-flow orifice, doing so before running Auto Pond is not recommended as this may impair the program's ability to optimize the pond configuration. The following general approach is suggested for designing a pond when there is a small value for the low end of the flow matching range:

1. First estimate the minimum pond volume allowing Auto Pond to freely determine the diameter and placement of all orifices.
2. Then manually accept all of the pond settings except low-flow orifice diameter. Set the low-flow orifice to the desired minimum size, after consulting the local municipal permitting agency.
3. Manually run the mitigated scenario as described on page 46 and review the Analysis screen to check if the revised mitigated flow still passes the flow-duration criteria for curve matching. If so, proceed with the pond design using the revised outlet.
4. If the revised design shows Fail scoring at one or more flow levels, excess flow durations may be reduced somewhat by reducing the depth of the pond which lowers the head above the orifice (SWMWW recognizes a practical minimum of 3 feet of live storage if pond shallowing is required at the minimum orifice size. As an alternative, further mitigation can be applied to the low-flow orifice flow by adding an additional infiltration measure downstream. This can be sized either approximately by estimating an average excess flow from the orifice or with the help of BAHM2023 by returning to the screen for the Pond characteristics and specifying a different Downstream Connection for the bottom orifice, which is then connected to an additional element. With this revision to the post project scenario, the Point of Compliance for the system would then be located at the downstream end of the additional low-flow mitigation.

Alternative Outlet Configurations

BAHM2023 has two default types of outlet configurations (multiple orifice or orifice plus weir notch) based on a standpipe riser structure detailed in the SMMWW. The entire standpipe is usually within a cylindrical enclosure or manhole to exclude trash and larger particles that could clog the outlet. The SMMWW notes that orifices can also be placed on a tee section or a vertical baffle within the same type of enclosure. An alternative configuration is a flat headwall with orifices and or notches, protected by racks or gratings. This may be fabricated from a large steel plate, similar in construction to the extended detention outlets specified in the Denver (Colorado) manual referenced below. This alternative outlet can be simulated in the BAHM2023 as a very large diameter standpipe, where the width of the top notch is equal to the overflow width at the top of the plate between its supports.

Drawdown Time and Considerations

Flow duration control facilities are designed to detain stormwater on-site for an extended period of time. The drawdown time is a concern to designers in relation to two areas of design besides hydromodification management¹⁶:

1. Standing water for extended periods provides a potential habitat in which mosquitoes can breed. Each Bay Area stormwater program has worked with its local mosquito abatement or vector control agencies to develop guidelines for stormwater facility design; these generally recommend that design detention times not exceed 72 hours, and under no circumstances should exceed 5 days. Provisions for access and inspection by vector control personnel are also required. See stormwater C.3 guidance documents at the weblinks under Additional Resources for details of local vector control provisions, which apply to both treatment measures and flow duration facilities.
2. Flood control design is intended to control peak flows for large sized storms (with expected recurrence intervals such as 15, 25 or 100 years). Flood control facilities typically require capture and detention of a specified volume of stormwater, which then is discharged out at flows that can be safely conveyed by downstream channels without undue risk of flooding. Flood control facilities usually are required to drain within 24 hours after the end of the design storm in order to be empty for the next storm event. This concern that flood control storage remain available for large events has led some flood control agencies to require that any storage volume for hydromodification control not be credited for flood control, a feature that is sometimes referred to as “dead storage”.

Although many factors affect the drawdown time, the suggestions below may help BAHM2023 users in evaluating these other requirements. If flow duration control is required for a project site, it is recommended that the design process start with by using BAHM2023 to obtain a preliminary design for the flow duration pond, vault, or tank. Then check the performance of the facility for vector control concerns, and against flood control design criteria as appropriate. The latter is typically based on the concept of a single empirical “design storm” which does not directly correspond to the flow duration approach using frequency analysis in a long-term simulation.

Vector Control

If the 3-day drawdown is seldom or never exceeded over the simulation period, then likelihood of mosquito breeding in the facility is very low and the design for the pond, vault or tank does not need to be modified. If a 5-day drawdown time is exceeded more than once or twice during the simulation, the system may need to be redesigned to reduce the drawdown time. The designer should consider additional reductions in impervious area and/or LID elements to help reduce the facility size.

¹⁶ Drawdown time also influences the effectiveness of a flow duration control facility for stormwater treatment; however, under the MRP, HM flow duration ponds, tanks, or vaults cannot be used as treatment facilities because detention basins are not considered LID treatment.

To evaluate the frequency and distribution of larger events in more detail, use the Hydrograph tool (page 140) to plot monthly peaks for several years at a time of the mitigated (post-project) scenario to get an idea of how often the discharge that corresponds to the 3-day drain time would be exceeded during warmer months, when mosquito development times are shortest.

Flood Control

Local flood control design criteria must be obtained from the appropriate agency, as well as any other policies or restrictions that may apply to drainage design. A single design storm event can be imported as a time series (page 67) and applied to the post-project scenario instead of the simulated precipitation record. If additional live storage is needed, it may be added to upper levels of the same facility or provided elsewhere on the site.

Additional Resources

Stormwater Programs have produced guidance documents for new and redevelopment projects in each county, which cover all “C.3” requirements including hydromodification management. These are available from local municipal permitting agencies and also on the following stormwater program websites:

Alameda Countywide Clean Water Program: www.cleanwaterprogram.org

San Mateo Countywide Water Pollution Prevention Program: www.flowstobay.org

Santa Clara Valley Urban Runoff Pollution Prevention Program: www.scvurppp.org

Contra Costa Clean Water Program (CCCWP): <https://www.cccleanwater.org/>

The BAHM2023 website includes links to BAHM2023 software and support documents and announcements about BAHM2023 updates and trainings:

<https://www.clearcreeksolutions.info/bahm-download-page> .

Guidance by Other Agencies

Some agencies in other parts of the US have developed extensive guidance for design of stormwater management measures. Two manuals are discussed below that provide detailed discussions or examples that may be helpful to users of BAHM, although the suitability of these recommendations for Bay Area conditions has not been verified. These documents can help provide context and ideas for users for BAHM, but adapting these ideas requires the exercise of professional engineering judgment. **Mention of the procedures and details in these documents does not imply any endorsement or guarantee that they will be appropriate for addressing the Hydromodification Management Standards in Bay Area jurisdictions.**

Stormwater Management Manual for Western Washington (SMMWW) was prepared by the Washington Department of Ecology for implementation in 19 counties of Western Washington. The latest (2019) edition in 5 volumes is on the Web at:

<https://apps.ecology.wa.gov/publications/SummaryPages/1910021.html>

Design recommendations from this manual were the basis for many features of the WWHM that have been carried over into BAHM. Portions of Volume 3 (Hydrology) that may be of interest to project designers include:

- Pages V4.1 through V4.7 illustrate several types of roof downspout controls, simple pre-engineered designs for infiltrating and/or dispersing runoff from roof areas in order to reduce runoff volume and/or increase potential groundwater recharge.
- Pages V1.4 to V1.6 discuss outlet control structures, their maintenance and source equations modeled into WWHM and BAHM
- Pages V5.4 to V5.5 regarding Infiltration Reduction Factor

Urban Storm Drain Criteria Manual by the Denver Urban Drainage and Flood Control District is on the Web at: <https://mhfd.org/resources/criteria-manual-volume-2/>
Volume 3 covers design of extended detention basins on pages 12-12 through 12-16.

APPENDIX E: BIORETENTION MODELING METHODOLOGY

Water Movement Through the Soil Column

Water movement through the soil column is dependent on soil layer characteristics and saturation rates for different discharge conditions.

Consider a simple two-layered bioretention facility designed with two soil layers with different characteristics. As water enters the facility at the top, it infiltrates into the soil based on the modified Green Ampt equation (Equation 1). The water then moves through the top soil layer at the computed rate, determined by Darcy's and Van Genuchten's equations. As the soil approaches field capacity (i.e., gravity head is greater than matric head), we can determine when water will begin to infiltrate into the second layer (lower layer) of the soil column. This occurs when the matric head is less than the gravity head in the first layer (top layer).

Since the two layers have different soil characteristics, water will move through the two layers at different rates. Once both layers have achieved field capacity then the layer that first becomes saturated is determined by which layer is more restrictive. This is determined by using Darcy's equation to compute flux for each layer at the current level of saturation. The layer with the more restrictive flux is the layer that becomes saturated for that time step. The next time step the same comparison is made.

The rate and location of water discharging from the soil layer is determined by the discharge conditions selected by the user.

There are four possible combinations of discharge conditions:

1. There is no discharge from the subsurface layers (except for evapotranspiration). This means that there is no underdrain and there is no infiltration into the native soil. Which this discharge condition is unlikely, we still need to be able to model it.
2. There is an underdrain, but no native infiltration. Discharge from the underdrain is computed based on head conditions for the underdrain. The underdrain is configured to have an orifice. (It is possible for the orifice to be the same diameter as the underdrain.) With a maximum of three soil layers determining head conditions for the orifice is complicated. Each modeled layer must overcome matric head before flow through the underdrain can begin. Once matric head is overcome by gravity head for all of the layers then the underdrain begins to flow. The flow rate is determined based on the ability of the water to move through the soil layers and by the discharge from the orifice, whichever is smaller. Head conditions are determined by computing the saturation level of the lowest soil layer first. Once the lowest soil layer is saturated and flow begins then the gravity head is considered to be at the saturation level of the lowest soil layer. Once the lowest soil layer is saturated completely then the head will include the gravity head from the next soil layer above until gravity head from all soil

layers is included. Gravity head from ponding on the surface is included in the orifice calculations only if all of the intervening soil layers are saturated.

3. There is native infiltration but no underdrain. Discharge (infiltration) into the native soil is computed based a user entered infiltration rate in units of inches per hour. Specific head conditions are not used in determining infiltration into the native soil. Any impact due to head on the infiltration rate is considered to be part of the determination of the native soil infiltration rate. Because it is possible to have a maximum of three soil layers, each modeled layer must overcome matric head before infiltration to the native soil can begin. Once matric head is overcome by gravity head for all modeled layers then infiltration begins at a maximum rate determined either by the ability of the water to move through the soil layers or by the ability of the water to infiltrate into the native soil, whichever is limiting.
4. There is both an underdrain and native infiltration. Underdrain flow and native infiltration are computed as discussed above. However, there is one other limitation to consider. In the case where the flow through the soil layer is less than the sum of the discharge through the underdrain and the native infiltration then the flow through the soil layer becomes the limiting flow and must be divided between the native infiltration and the underdrain. This division is done based on the relative discharge rates of each.

Note that wetted surface area can be included in the discharge calculations by adding the infiltration through the wetted surface area to the lower soil layer and the upper surface layer individually. This is done by computing the portion of the wetted surface area that is part of the upper surface layer and computing the infiltration independently from the portion of the wetted surface area that is part of the lower soil layers.

Water Movement Equations

There are several equations used to determine water movement from the surface of the bioretention facility, through the soil layers, and into an underdrain or native infiltration. The water movement process can be divided into three different zones:

- 1) Surface ponding and infiltration into the top soil layer (soil layer 1)
- 2) Percolation through the subsurface layers
- 3) Underdrain flow and native infiltration

Surface ponding and infiltration into the top subsurface layer

The modified Green Ampt equation (Equation 1) controls the infiltration rate into the top soil layer:

$$f = K \left(1 + \frac{(\phi - \theta)(d + \varphi)}{F} \right) \quad \text{(Equation 1; Ref: Rossman, 2009)}$$

f = soil surface infiltration rate (cm/hr)

ϕ = soil porosity of top soil layer

θ = soil moisture content of top soil layer

φ = suction head at the wetting front (cm)

F = soil moisture content of the top soil layer (cm)

d = surface ponding depth (cm)

K = hydraulic conductivity based on saturation of top soil layer (cm/hr)

K (relative hydraulic conductivity) can be computed using the following Van Genuchten approximation equation:

Van Genuchten approximation of relative hydraulic conductivity

$$\frac{K(\theta)}{K_{sat}} = \left(\frac{\theta - \theta_r}{\phi - \theta_r} \right)^{1/2} \left[1 - \left(1 - \left(\frac{\theta - \theta_r}{\phi - \theta_r} \right)^{1/m} \right)^m \right]^2 \quad \text{(Equation 2; Ref: Blum et al, 2001)}$$

where $K(\theta)$ = relative hydraulic conductivity,

K_{sat} = saturated hydraulic conductivity,

θ = water content, θ_r = residual water content,

ϕ = porosity, α = constant, n = constant, m = constant

A few issues arise when dealing with multiple subsurface soil layers. The K value used in Equation 1 must be computed from the top soil layer. Infiltration into the upper soil layer must not exceed the lesser of the maximum percolation rates for each of the soil layers. Finally, the rate of percolation of the top layer may be reduced because the layer or layers beneath the top layer cannot accept the percolation flux because of existing saturation levels.

Percolation through the subsurface layers

Water storage and movement through the three subsurface layers will be computed using Darcy's equation as shown below:

$$q = -K \frac{\partial h}{\partial z} \quad (\text{Equation 3})$$

Where:

q = Darcy flux (cm/hr)

K = hydraulic conductivity of the porous medium (cm/hr)

h = total hydraulic head (cm)

z = elevation (cm)

The total head, h , is the sum of the matric head, ψ , and the gravity head, z :

$$h = \psi + z \quad (\text{Equation 4})$$

Substituting for h yields:

$$q = -K \frac{d(\psi + z)}{dz} \quad (\text{Equation 5})$$

Hydraulic conductivity and matric head vary with soil moisture content. These values can be computed by solving the Van Genuchten's equation (Equation 6) for both values.

Note that $\psi = 0$ when the soil is saturated.

Van Genuchten Equation to calculate total head

$$h = -\frac{1}{\alpha} \left[\frac{1}{SE^{1/m}} - 1 \right]^{1/n} + z \quad \text{(Equation 6; Ref: Blum et al, 2001)}$$

where h = total hydraulic head, α = constant, SE = effective saturation,
 m = constant, n = constant, and z = elevation head

Effective saturation (SE) can be computed using the following Van Genuchten equation:
 Van Genuchten Equation to calculate effective saturation

$$\frac{\theta - \theta_r}{\phi - \theta_r} = \left[\frac{1}{1 + (\alpha\psi)^n} \right]^m = SE \quad \text{(Equation 7; Ref: Blum et al, 2001)}$$

where θ = water content, θ_r = residual water content,
 ϕ = porosity,
 α = constant = $y_b - 1$,
 n = constant = $\lambda + 1$,
 m = constant = $1 - \frac{1}{\lambda + 1}$,
 λ = pore size distribution index,
 y_b = bubbling pressure
 ψ = pressure head = $h - z$, h = total hydraulic head,
 z = elevation head, and SE = effective saturation

Ignoring z (elevation head) results in $h = hm$ (matric head).

Evapotranspiration from the Soil Column

Evapotranspiration is an important component of the bioretention facility's hydrologic processes. Evapotranspiration removes water from bioretention surface ponding and the soil column during non-storm periods. The routine will satisfy potential evapotranspiration (PET) demands in the same sequence as implemented in HSPF:

1. Water available from vegetation interception storage
2. Water available from surface ponding
3. Water available from the bioretention soil layers (top layer first)

Water will be removed from vegetation interception storage and surface ponding and the bioretention soil layers (starting at the top layer) down to the rooting depth at the potential rate. Water is taken from the soil layers below the rooting depth based on a percentage factor to be determined. Without this factor there will be no way to remove water from below the rooting depth once it becomes completely saturated.

References

Blum, V.S., S. Israel, and S.P. Larson. 2001. *Adapting MODFLOW to Simulate Water Movement in the Unsaturated Zone*. MODFLOW 2001 and Other Modeling Odysseys, International Groundwater Modeling Center (IGWMC), Colorado School of Mines, Golden, Colorado, September 11-14, 2001. In MODFLOW 2001 and Other Modeling Odysseys, Proceedings. pp.60-65.

Rossman, L.A. 2009. *Modeling Low Impact Development Alternatives with SWMM*. Presented at CHI International Stormwater and Urban Water Systems Conference, Toronto, Ontario, Canada, February 20, 2009.

APPENDIX F: PRECIPITATION DATA

Information on the precipitation gages, location, and period of record used in BAHM2023 is provided in the following table:

Gage Name	County	Lat/Long	Dates of Record	Years of Record
Berkeley	Alameda	37.8836, -122.22	10/1/1959 - 9/30/2022	63
Brentwood	Contra Costa	37.92, -121.678	10/1/1959 - 9/30/2021	63
Dublin Fire	Alameda	37.7313, -121.928	10/1/1973 - 9/30/2021	48
Flood Control District (WC)	Contra Costa	37.988, -122.085	10/1/1959 - 9/30/2021	62
Livermore	Alameda	37.6547, -121.742	10/1/1959 - 9/30/2022	63
Los Medanos	Contra Costa	37.9974, -121.8564	10/1/1974 - 9/30/2021	47
Martinez	Contra Costa	37.977, -122.178	10/1/1959 - 9/30/2021	62
Morgan Hill	Santa Clara	Discontinued*	10/1/1959 - 9/30/2022	63
Newark	Alameda	Discontinued*	10/1/1959 - 9/30/2022	63
Orinda Fire	Contra Costa	37.89957, 122.17067	10/1/1973 - 9/30/2021	48
Saint Mary's	Contra Costa	37.842, -122.107	10/1/1972 - 9/30/2021	49
San Francisco	San Mateo	37.617, -122.383	10/1/1959 - 9/30/2022	63
San Jose	Santa Clara	37.35, -121.9	10/1/1959 - 9/30/2022	63

*The San Jose gage data was used to extend the record of the discontinued gages.

Precipitation gages are scaled based on the average annual depth of rainfall. The selected location is scaled based on the isopluvial map of the average annual rainfall depths. The rainfall is then scaled according to the ratio of the average annual rainfall depth at the gage location to that of the site location.